


Multifors 2

Bench-Top Bioreactor - Version for Microorganisms

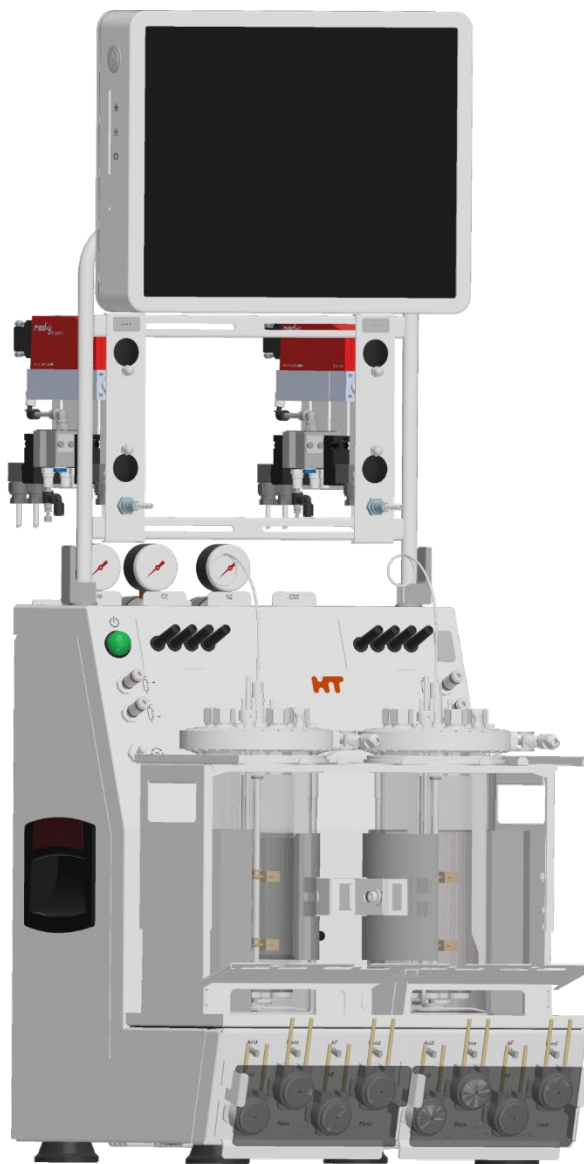

INFORS HT
Headoffice, Switzerland

Rittergasse 27
CH-4103 Bottmingen
T +41 (0)61 425 77 00
F +41 (0)61 425 77 01
info@infors-ht.com
service@infors-ht.com

INFORS HT, Germany
Dachauer Str. 6
D-85254 Einsbach
T +49 (0)8135 8333
F +49 (0)8135 8320
infors.de@infors-ht.com

INFORS HT, UK
The Courtyard Business Centre
Dovers Farm, Lonesome Lane,
Reigate
Surrey, RH2 7QT, UK
T +44 (0)1737 22 31 00
F +44 (0)1737 24 72 13
infors.uk@infors-ht.com

INFORS HT, France
2, rue du Buisson aux Fraises
Bâtiment D13
F-91300 Massy
T +33 (0)1 69 30 95 04
F +33 (0)1 69 30 95 05
infors.fr@infors-ht.com

INFORS HT, Benelux
Markweg 9-A, NL-6883 JL
Velp (GLD)
P.O. Box 125, NL-6880 AC
Velp (GLD)
T +31 (0)26 369 31 00
F +31 (0)26 369 31 09
infors.bnl@infors-ht.com

INFORS HT, USA
9070 Junction Drive, Suite D
Annapolis Junction, MD20701
T +1 301 362 3710 /
T +1 855 520 7277 (toll-free USA)
F +1 301 362 3570
infors.usa@infors-ht.com

INFORS, HT, Canada
8350 rue Bombardier
Anjou, Quebec
Canada H1J 1A6
T +1 514 352 5095
F +1 514 352 5610
infors.ca@infors-ht.com

INFORS HT, China
Room 503, C Hall,
M8 Office Building
No. 1 Jiuxianqiao East Road
Chaoyang District, Beijing
China 100015
T +86 10 51652068
F +86 10 64390585
info@infors-ht.com.cn

INFORS HT Southeast Asia
16, 1st Floor, Taman City
MY-51200 Kuala Lumpur
Malaysia
T +603 625 771 81
F +603 625 067 48
info@infors-ht.com.my

INFORS HT, Latin America
Rua Dr. Alceu de Campos
Conjunto 205
CEP: 04544-000
São Paulo – SP
Brasil
T +55 (11) 95304-0201
F +55 (11) 98585-5334
Infors.br@infors-ht.com

**Contact details of our local dealers worldwide can be found
on our website.**

www.infors-ht.com



Engineering and production in Switzerland

Table of Contents

1	General Information	8
1.1	About this Manual	8
1.2	Explanation of Special Notices	9
1.2.1	Warning Notices	9
1.2.2	Other Notices.....	9
1.3	Device Identification (Standard Identification Plate)	10
1.4	Declaration of Conformity	10
1.5	Customer Service and Services	10
2	Safety and Responsibility	11
2.1	Intended Use, Incorrect Use and Misuse	11
2.2	Qualified Personnel	12
2.2.1	Provider	12
2.2.2	User	12
2.2.3	Operator	13
2.3	Unauthorised Persons	14
2.4	Responsibility of the Provider	14
2.5	General Hazards.....	15
2.5.1	Electrical Current.....	15
2.5.2	Unauthorised Spare Parts and Accessories	15
2.6	Particular Hazards	15
2.6.1	Hot Surfaces.....	16
2.6.2	Dangerous Gases	16
2.6.3	Flammable or Explosive Substances	16
2.6.4	Corrosive or Toxic Substances	16
2.6.5	Bioactive Substances or Pathogenic Organisms	17
2.6.6	Overpressure or Vacuum	17
2.7	Warning Symbols on the Device.....	17
2.8	Declaration of Decontamination.....	18
3	Setup and Function.....	19
3.1	Basic Unit.....	19
3.1.1	Power Switch.....	20
3.1.2	Pumps	20
3.1.3	Identification Plate	22
3.1.4	Mains Connection and Device Fuses.....	22
3.1.5	Water Connections.....	22
3.1.6	Gas Connections.....	23
3.1.7	Gassing Connection (Sparger).....	24
3.1.8	Sensor Connections (Sensor Cables).....	25
3.1.9	Connections Exit Gas Cooler and Valves for Water Flow	25

Table of Contents

3.2	Operating Panel	26
3.3	Culture Vessel	27
3.3.1	Ports in the Vessel Top Plate and their Configuration	28
3.3.1.1	Vessel Top Plate, DN 70/55	29
3.3.1.2	Vessel Top Plate, DN 70	30
3.3.1.3	Vessel Top Plate, DN 90	31
3.4	Temperature Control System	32
3.5	Stirrer	33
3.6	Gassing System	35
3.7	Exit Gas	36
3.8	pH Control	37
3.9	pO ₂ Control	38
3.10	Antifoam Control	41
4	Options	42
4.1	Pump(s)	42
4.2	Balances	42
4.3	Level Detection	43
4.4	Exit Gas Analysis	44
4.4.1	Measurement Systems (Gas Sensors)	44
4.4.2	Connecting the Gas Sensors	44
4.4.3	Calibration	45
4.4.4	Replacing the BlueVary Gas Sensor Cartridge	45
4.5	Multiplexer (Gas Switching Module)	46
4.6	Turbidity Measurement	46
4.6.1	Calibrating the Sensor	48
4.6.2	Mounting the Sensor	48
4.6.3	Interferences Turbidity Measurement	49
4.7	Permissive Measurement	50
4.8	Redox Measurement	50
4.9	Conductivity Measurement	51
5	Accessories	53
5.1	Vessel Holder	54
5.2	Vessel Adapter	56
5.3	Sampling System Super Safe Sampler	56
5.4	Sparger	60
5.5	Impellers	61
5.6	Immersion Pocket for Temperature Sensor (Pt100)	61
5.7	Baffles	62
5.8	Blanking Plugs	63

Table of Contents

5.9	Addition Port Adapters	64
5.10	Inoculation Needles	64
5.11	Septum Collars	65
5.12	Dip Tubes	66
5.13	Clamping Adapters	68
5.14	Sensor Holder	69
5.15	Exit Gas Cooler	70
5.16	Adapter Sleeve	72
5.17	Reagent Bottles	72
5.18	Antifoam Sensor	74
5.19	Pump Heads	75
5.20	Sterile Filters	75
5.21	O-Rings and Gaskets	77
5.22	Hoses and Hose Accessories	77
5.23	Tools and Inoculation Accessories	78
6	Transport and Storage	79
6.1	Transport	79
6.2	Storage	80
7	Installation and Commissioning	81
7.1	General Location Requirements for Installation	81
7.2	Minimum Distances	82
7.3	Power Supply	82
7.4	Water Supply and Return	82
7.5	Gas Supply	83
7.6	Exit Gas	83
7.7	Test Run	84
7.7.1	Preparation Test Run	84
7.7.2	Cooling System	85
7.7.3	Stirring	86
7.7.4	Heating and Adjusting Temperature	86
7.7.5	Gassing	87
7.7.6	End of Test	87
8	Before Cultivation	88
8.1	Preparing and Autoclaving the Culture Vessel	88
8.1.1	Checking Gaskets (O-Rings)	88
8.1.2	Mounting the Bearing Holder in the Top Plate	89
8.1.3	Mounting the Addition Port Adapters and Hose Holder	90
8.1.4	Mounting the Stirrer Shaft	91
8.1.5	Mounting the Baffles	92

Table of Contents

8.1.6	Mounting the Impeller, Flow Deflector and Magnetic Coupling	94
8.1.7	Checking the Fit of the Centering Bearing of the Stirrer Shaft.....	96
8.1.8	Mounting Dip Tubes and Spargers.....	97
8.1.9	Positioning the Sparger in the Vessel	99
8.1.10	Adjusting the Longitudinal Play of the Stirrer Shaft	99
8.1.11	Moistening/Filling the Culture Vessel	101
8.1.12	Putting on the Vessel Top Plate, Fastening with Clamping Ring.....	102
8.1.13	Inserting the Culture Vessels into the Vessel Holder	104
8.1.14	Mounting the Immersion Pocket for Temperature Sensor (Pt100).....	104
8.1.15	Mounting the Adapter Sleeve	105
8.1.16	Mounting the Exit Gas Cooler.....	105
8.1.17	Mounting the Blanking Plugs	108
8.1.18	Equipping the Port with a Septum Collar and Septum for Inoculation.....	109
8.1.19	Preparing the Dip Tube/Addition Port Adapter for Inoculation	110
8.1.20	Preparing the Sensors	110
8.1.20.1	Calibrating the pH Sensor	111
8.1.20.2	Mounting a Sensor into a 12 mm Port.....	112
8.1.20.3	Mounting Sensors with Sensor Holder	112
8.1.20.4	Mounting the Antifoam Sensor...	114
8.1.21	Preparing the Super Safe Sampler.....	117
8.1.22	Mounting the Sparger Hose and the Inlet Air Filter	119
8.1.23	Preparing the Gassing Hose Line on the Basic Unit	120
8.1.24	Calibrating the Pumps	120
8.1.25	Preparing the Reagent Bottles, Pumps and Hoses.....	121
8.1.26	Sterile Hose Connections	123
8.1.27	Removing the Pump Heads.....	124
8.1.28	Checklist Before Autoclaving	125
8.1.29	Autoclaving	126
8.2	Connecting the Culture Vessel and Preparing the Cultivation	127
8.2.1	Fixing the Culture Vessels to the Basic Unit	127
8.2.2	Mounting the Pump Heads	128

Table of Contents

8.2.3	Filling the Reagent Hoses	129
8.2.4	Connecting the Gassing	130
8.2.5	Connecting the Exit Gas Cooler	131
8.2.6	Filling the Culture Vessel.....	132
8.2.7	Connecting the Temperature Sensor (Pt100)	132
8.2.8	Connecting the Antifoam Sensor.....	133
8.2.9	Connecting the pH Sensor	133
8.2.10	Connecting the pO ₂ Sensor.....	134
8.2.11	pO ₂ Sensor (Analog, Polarographic) Polarisation	135
8.2.12	Calibrating the pO ₂ Sensor.....	135
8.2.13	Checking the Hoses and Hose Connections	135
9	Cultivation.....	136
9.1	Preparing the Medium	136
9.2	Sampling	137
9.3	Inoculation.....	140
9.3.1	Inoculation with a Syringe	141
9.3.2	Inoculation Using Dip Tube / Addition Port Adapter	141
9.4	Harvest.....	142
9.5	Emptying the Culture Vessel	143
9.6	Emptying the Reagent Hoses	143
9.7	Switching off the Device	144
9.8	Autoclaving the Culture Vessel after Cultivation.....	144
10	Cleaning and Maintenance.....	146
10.1	Cleaning Agent and Disinfectant	146
10.2	Cleaning the Culture Vessel - Routine Cleaning	147
10.3	Removing the Vessel Top Plate and Accessories.....	148
10.3.1	Removing the Exit Gas Cooler	148
10.3.2	Removing the Sensors	150
10.3.3	Removing Hoses, Filters and Pump Heads	151
10.3.4	Removing Blanking Plugs	152
10.3.5	Removing the Septum Collar and the Septum	152
10.3.6	Removing the Vessel Top Plate.....	153
10.3.7	Removing the Immersion Pocket for Temperature Sensor (Pt100).....	153
10.3.8	Removing the Sparger and Dip Tube.....	154
10.3.9	Removing the Baffles	154

Table of Contents

10.3.10	Removing the Hose Holder and Addition Port Adapters	155
10.3.11	Removing the Stirrer Shaft	155
10.3.12	Removing the Magnetic Coupling, Flow Deflector and Impeller	156
10.3.13	Removing the Bearing Holder	158
10.4	Cleaning and Storing Individual Parts.....	159
10.5	Cleaning the Sensors.....	160
10.6	Cleaning the Hoses and Pump Heads.....	160
10.7	Cleaning the Super Safe Sampler	161
10.8	Cleaning the Magnetic Coupling	161
10.9	Cleaning the Basic Unit and Operating Panel	163
10.10	Maintenance Plan	163
10.11	Decalcifying the Device.....	165
10.12	Replacing the Centering Bearing	166
11	Interferences	167
11.1	Interferences Basic Unit and Operating Panel.....	167
11.2	Drive System Interferences.....	168
11.3	Interferences Temperature Control System.....	169
11.4	Interferences Gassing System.....	170
11.5	Interferences pH Control	171
11.6	Interferences pO ₂ Control.....	173
11.7	Interferences Antifoam or Level Sensor and Antifoam Pump	174
11.8	Interferences Feed and Pump	175
11.9	Replacing Device Fuses	175
11.10	Behavior in Case of Power Interruption	176
11.11	Returning for Repair.....	176
12	Disposal.....	177
13	Technical Data	178
13.1	Dimensions	178
13.1.1	Master Device and Satellite Devices	178
13.1.2	Culture Vessels in Vessel Holder	179
13.2	Weights	180
13.3	Connection Values	180
13.3.1	Electrical	180
13.3.2	Water IN.....	181
13.3.3	Water OUT.....	181
13.3.4	Gas(es) IN	181
13.3.5	Exit Gas	181
13.4	Specifications	182

Table of Contents

13.4.1	Operating Panel	182
13.4.2	Culture Vessels	182
13.4.3	Stirrer	183
13.4.4	Temperature	184
13.4.5	Gassing	184
13.4.6	Antifoam	185
13.4.7	pH Control	185
13.4.8	pO ₂ Control	186
13.4.9	Pumps	187
13.5	Operating Conditions	188
13.6	Emissions	188
13.7	Auxiliary Supplies	188
14	EC-Declaration of Conformity	189

General Information

1 General Information

1.1 About this Manual

This manual enables the safe and efficient handling of the device.

All the information and instructions in this operating manual comply with the current standards, legal regulations, the latest technological and scientific developments and the knowledge gained from the manufacturer's many years of experience in this field.



This operating manual is a component part of the device. It must be kept near to the device and must be accessible to the operators at all times.

The users must read the operating manual thoroughly and fully understand its contents before beginning any work.

Adhering to all the safety and operating instructions in this manual is essential to ensure that work is carried out safely.

The scope of delivery may differ from the explanations, descriptions and figures in this operating manual due to special designs, additional options specified on ordering and the latest technical/mechanical modifications.

This manual contains illustrations to aid general understanding. These may differ from the actual device as supplied.

1.2 Explanation of Special Notices

1.2.1 Warning Notices

Warning notices in this manual are indicated by a colored bar and begin with a signal word that signifies the degree of the hazard.



WARNING

The signal word "WARNING" indicates a potentially dangerous situation that may result in severe or even fatal injuries if not avoided.



CAUTION

The signal word "CAUTION" indicates a potentially dangerous situation that may result in minor injuries if not avoided.

1.2.2 Other Notices



ATTENTION

The word "ATTENTION" on a blue bar indicates a situation that may result in significant damage to property if not avoided.




INFORMATION

Texts located below a grey bar bearing the notice "INFORMATION" provide useful tips and recommendations for ensuring efficient, fault-free operation of the device.

General Information

1.3 Device Identification (Standard Identification Plate)

The identification plate is designed to allow clear identification of the device. It contains the following information:

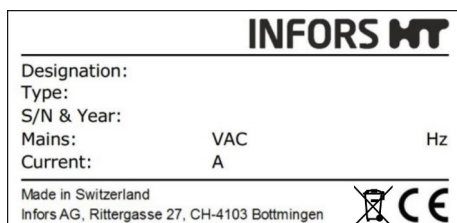

- Manufacturer name
- Designation = Category of device
- Type = Device type (name)
- S/N = Serial number
- Year = Year of manufacture
- Mains = Nominal voltage and frequency
- Current = Current consumption
- Manufacturer address
- WEEE marking
- CE marking

1.4 Declaration of Conformity

The device is in compliance with the essential requirements of the following Directives:

- Directive 2006/42/EC on Machinery
- EMC Directive 2014/30/EU

The Declaration of Conformity according to Directive 2006/42/EC on Machinery, annex II 1 A is attached to the operating manual, refer to chapter "EC-Declaration of Conformity".

1.5 Customer Service and Services

Our Customer Service is at your disposal for technical advice and specialist enquiries. For contact information, see page 2.

Due to their familiarity with the potential applications of the device, the Customer Service team is able to provide information on whether the device can be used for a specific application or modified to handle the planned process.

Furthermore, our colleagues are always interested in new information and experiences resulting from user's applications for the device that may be valuable for the continued development of our products.

2 Safety and Responsibility

This section describes general considerations relating to user safety that must be taken into account when working with the device.

In the remaining sections, warning notices are used only to highlight particular hazards directly arising from the actions being described in the section in question.



It is essential to read the operating manual carefully – especially this section and the warning notices in the text – and to follow the instructions therein.

This section also refers to areas that are the responsibility of the provider due to certain risks arising from particular applications for which the device is used deliberately and with full awareness of the associated risks.

2.1 Intended Use, Incorrect Use and Misuse

The bench-top bioreactor Multifors 2 from INFORS HT is designed especially for running bio processes with microorganisms or animal cells for research and development in a biotechnology laboratory.

The device is designed and constructed exclusively for the intended use described above.

Intended use also includes following all the instructions in this operating manual, especially those relating to:

- The installation site
- User qualifications
- Correct operation and maintenance
- The use of undamaged tubing and glass vessels

Any failure to observe the requirements specified in this manual shall be deemed incorrect use.

Any use of the device outside the scope of the intended use as described above shall be deemed misuse.

This also applies to applications for which the device is not designed, such as the use or production of explosive gases, which is not permitted because the device is not explosion-proof.

Safety and Responsibility

For use for special applications not covered by conventional, intended use, the device must be modified and certified accordingly by the manufacturer.

Any use of the device outside of a biotechnology laboratory, i.e. in any environment in which the conditions required for the safety of the users cannot be fulfilled or cannot be fulfilled to their full extent, shall also be deemed misuse.

2.2 Qualified Personnel

Due to the complexity of the device and the potential risks arising from its operation, the device may only be used by qualified, specialist personnel.

2.2.1 Provider

The term “provider” applies to all persons who are responsible for making the device and the necessary infrastructure available. These persons may also be included in the group of people known as “users”, though this is not always the case.

Irrespective of whether a provider is a member of the company's board of management or a supervisor, they bear a special level of responsibility with regard to the processes and the qualification and safety of the users.

2.2.2 User

General

The term “user” applies to all persons who come into contact with the device in any way and perform work on or with it. This primarily applies to the following activities, which can be performed by the manufacturer's own specialists or a variety of other persons (it is not always possible to distinguish clearly between the different types of person):

- Assembly, installation and commissioning
- Definition and preparation of the process
- Operation
- Troubleshooting and remedying of faults
- Maintenance and cleaning (autoclaving, if necessary)
- Service work and repairs
- Disassembly, disposal and recycling

Safety and Responsibility

Qualified personnel

On account of their specific education, training and – in many cases – experience, the qualified personnel required for this work are able to recognise risks and respond accordingly to potential hazards.

The qualified personnel (either internal or external) who cannot be categorised under the separate “operators” group are made up of the following groups of persons:

- Electricians (electrical engineers)
- Decontamination specialists
- Repair specialists
- Specialists in disassembly and (environmentally friendly) disposal
- Recycling specialists

2.2.3 Operator

The “operators” are a specific sub-group of users distinguished by the fact that they work with the device. They are the true target audience for this operating manual.

Qualified technicians

Only technicians who have been trained for working in a biotechnology laboratory can be considered for the role of operator. These include:

- Process technicians in the fields of biotechnology and chemistry
- Biotechnologists (biotechnicians)
- Chemists with a specialisation in biochemistry; chemists in the field of organic chemistry or biochemistry
- Life scientists (biologists) with special education in cytology, bacteriology, molecular biology, genetics, etc.
- Lab assistants (lab technicians) from various fields

In order to be classed as a “sufficiently qualified technician” for the operation of the device, the persons in question must have received thorough training and have read and understood the operating manual.

The operator must be informed in a training session provided by the provider of the tasks delegated to the operator and the potential risks of improper conduct. Tasks that go beyond the scope of operation under normal conditions may only be performed by the

Safety and Responsibility

operator if this is specified in the manual and the provider has explicitly entrusted said tasks to the operator.

Technicians in training

Persons in this group who are undergoing training or apprenticeships are only permitted to use the device under supervision and in accordance with the instructions of a trained and qualified technician.

2.3 Unauthorised Persons

The term “unauthorised persons” applies to all persons who can access the work area but are not qualified to use the device in accordance with the aforementioned requirements.

Unauthorised persons are not permitted to operate the device or use it in any other way.

2.4 Responsibility of the Provider

The device is used for industrial and scientific purposes. As such, the provider of the device is individually liable with regard to the legal requirements relating to occupational health and safety in a biotechnology laboratory. In particular:

- The provider is responsible for ensuring that the work and environmental regulations applicable in a biotechnology laboratory are observed.
- The provider must ensure that the device remains in safe and proper working condition throughout its entire term of use.
- The provider must ensure that all safety equipment is fully functional and is not disabled.
- The provider must ensure that the device is only worked on by qualified users, and that said users receive sufficient training.
- The provider must ensure that the protective equipment required for working with the device is provided and worn.
- The provider must ensure that this operating manual remains in the immediate vicinity of the device throughout its entire term of use.

2.5 General Hazards

This section covers general hazards and residual risks that are always present when using the device in accordance with normal, intended use.

The following notices are general in nature. As such, with a few exceptions they are not repeated in the remaining sections.

2.5.1 Electrical Current



The device runs on electrical power. There is an immediate risk of fatal injury if contact is made with live parts.

The following points must be observed in order to avoid the risk of fatal injury:

- In case of damage to insulation, disconnect the device from the power supply immediately and arrange for it to be repaired.
- Disconnect the device from the power supply before commencing any work on the electrical system.
- Always use qualified electricians for any work on the electrical system.
- Keep moisture away from live parts. It may lead to a short circuit.

2.5.2 Unauthorised Spare Parts and Accessories



Incorrect or imitated spare parts and accessories as well as spare parts or accessories that have not been authorised by the manufacturer represent a significant safety risk. As such, we recommend procuring all spare parts and accessories from an authorised dealer or directly from the manufacturer. For the contact details of the manufacturer's representatives, see page 2.

2.6 Particular Hazards

This section covers particular hazards and residual risks that may arise when using the device for special applications in accordance with normal, intended use.

Since the use of the device for such applications is deliberate, it is the responsibility of the operators and the provider to ensure that all personnel are protected from potential damage to health. The

Safety and Responsibility

provider is responsible for ensuring that the appropriate protective equipment for such applications is provided, and that the necessary infrastructure is in place.

2.6.1 Hot Surfaces



For processes that are carried out with temperatures over 55 °C, there is a danger of burns on hot surfaces.

Since the device is intended for applications at high temperatures, it is the responsibility of the users to ensure that they have sufficient protection.

The thermal block gets hot during operation. There is a risk of burns, if touched.

2.6.2 Dangerous Gases



The use or production of dangerous gases i.e. toxic or asphyxiant gases entails a significant health risk, especially in enclosed spaces.

In order to prevent high emissions of dangerous gases, the following measures must be taken:

- The gas connections on the device must be checked before any cultivation processes using dangerous gases are initiated.
- The gaskets on the device must be checked at regular intervals and replaced if necessary.
- Siphon off exit gas safely.

2.6.3 Flammable or Explosive Substances



The use or production of flammable or explosive substances is not covered under “intended use” of the device, as the device is not explosion-proof.

If the provider intends to use the device for such purposes, he must check its suitability for the planned application with the responsible local authorities.

2.6.4 Corrosive or Toxic Substances



The use or production of corrosive or toxic substances entails a significant health risk. As such, special measures must be taken to protect the users for such applications.

Safety and Responsibility

Since the device is used deliberately for such applications, it is the responsibility of the users to ensure that they have sufficient protection.

2.6.5 Bioactive Substances or Pathogenic Organisms



The use or production of bioactive substances, pathogenic organisms or genetically modified cultures entails a significant health risk. As such, special measures must be taken to protect the users for such applications.

Since the device is used deliberately for such applications, it is the responsibility of the users to ensure that they have sufficient protection.

2.6.6 Overpressure or Vacuum



Glass vessels may break or shatter when subjected to overpressure or vacuums.

2.7 Warning Symbols on the Device

The following warning symbols (stickers) are attached to the device:

Position

Thermal block



WARNING

Illegible or missing warning symbols on the device will lead to the user being exposed to risks that the warning symbols in question were designed to make him or her aware of.

It is the provider's responsibility to ensure that all the stickers with warning symbols on the device are always intact.

Safety and Responsibility

2.8 Declaration of Decontamination

When returning the device for repair, disassembly or disposal, it is required for the safety of all parties involved and because of legal provisions that a lawful declaration of decontamination is present.

The following must be observed if this is the case:


- The device, the component part or accessory must be entirely decontaminated before sending to the manufacturer
- The provider is therefore required to completely and truthfully fill out a declaration of decontamination, and have it signed by the person responsible.
- **The declaration of decontamination must be affixed on the outer packaging in which the device is sent back.**
- These forms can be obtained from the licensed dealer or the manufacturer. See address on page 2.

Important notice

If the return shipment is not accompanied by a signed and complete declaration of decontamination or it is not affixed to the outer packaging, the shipment will be returned unopened to the sender at their expense (see also T&C).

3 Setup and Function

3.1 Basic Unit

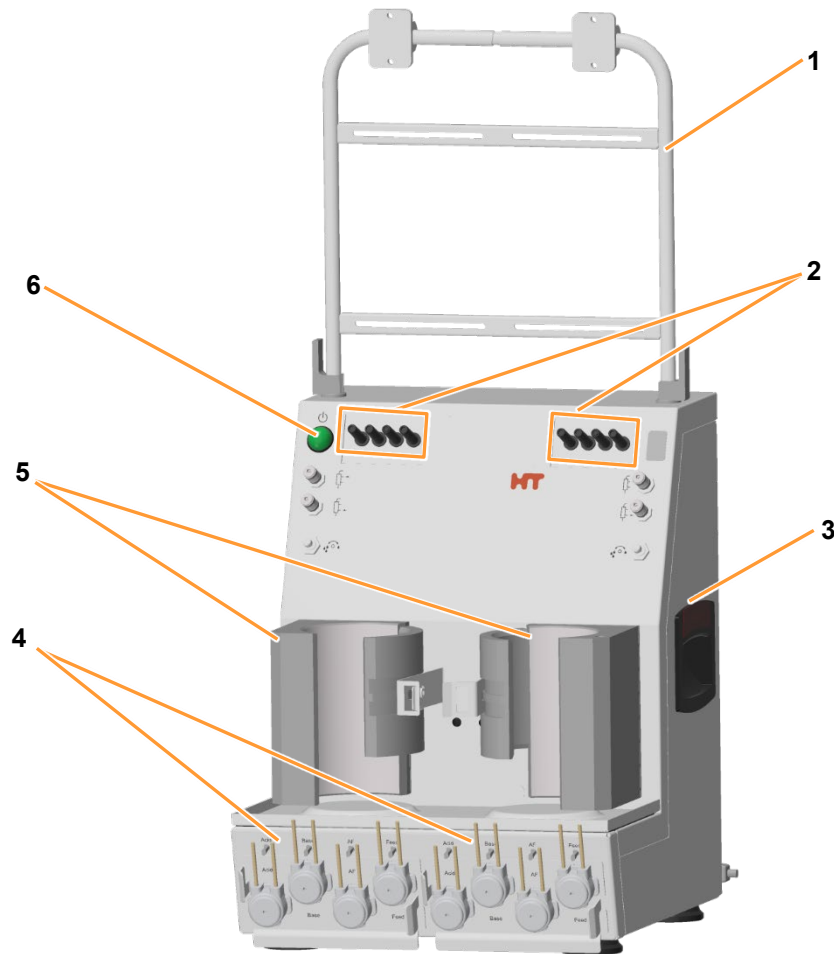

- | | | | |
|---|--|---|---------------|
| 1 | Device frame with holder for gassing unit(s) ¹⁾ and operating panel | 4 | Pumps |
| 2 | Sensor cables | 5 | Thermal block |
| 3 | Hand grip basic unit (1 x left, 1 x right) | 6 | Power switch |

¹⁾ Depending on the chosen gassing strategy this can be rotameter(s), mass flow controller(s), solenoid valve(s)


The whole measurement and control technology is integrated in the basic unit. One operating panel with touch screen software can be used to control up to six bioreactors (culture vessels)

Setup and Function

individually or in parallel, see also chapter “Operating Panel”. This means, one basic unit serves as the master device and can control up to two more basic units, referred to as satellite devices.

Two culture vessels of the same size placed in a vessel holder can be connected to the basic unit.

3.1.1 Power Switch

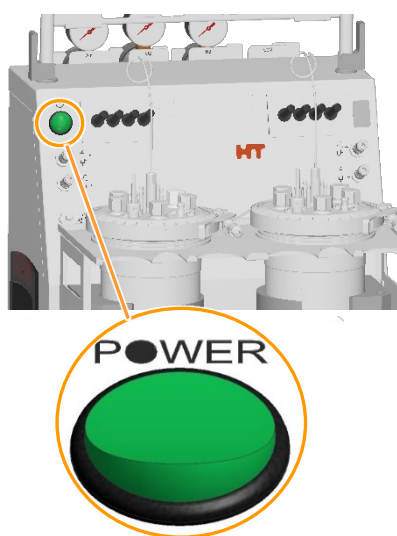

The power switch, a green rocker switch, is located at the top left on the front of the basic unit. It is labelled with **POWER** and lights up as soon as the device is switched on. In addition to normal switching on and off, the power switch also serves as an emergency switch.



INFORMATION

In the event of an emergency shutdown via the power switch during a running Batch (process), all settings are saved. After switching on via the power switch, the Batch continues with the same settings as before the emergency shutdown. This is also the case if the Batch is controlled via eve®, the platform software for bioprocesses.

3.1.2 Pumps



Reagents and nutrient solution are added via four peristaltic pumps per culture vessel. The pumps are driven by stepper motors. The drive shafts of the pumps are located at the bottom of the front side of the basic unit. The default direction of rotation is counter-clockwise. The pumps can be operated manually with rocker switches located above the drive shafts. They are labelled from left to right):


- **Acid**
- **Base**
- **AF (Antifoam)**
- **Feed**

Setup and Function



When the device is switched on, pumps can be manually operated via the rocker switches as follows:


- Push and hold the rocker switch to the right:
The pump drive shaft turns counter-clockwise.
- Push and hold the rocker switch to the left:
The pump drive shaft turns clockwise.

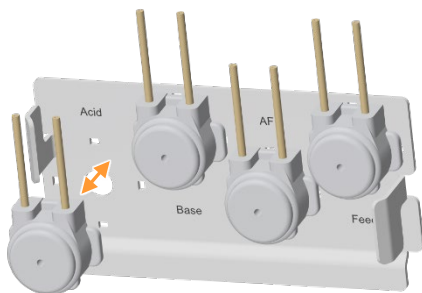

The autoclavable pump heads are latched onto a mounting plate. The mounting plate is identically as the drive shafts labelled with the pump names.



The pump heads together with the mounting plate can be plugged onto or pulled off the drive shafts.

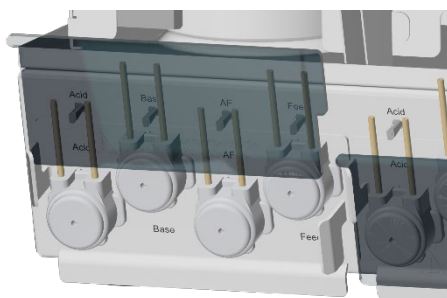

A transparent, not autoclavable (!) cover plate made of plexiglass can be inserted into the holder of the mounting plate for protection during operation.


Setup and Function

3.1.3 Identification Plate

The identification plate is located on the rear of the basic unit.

The data provided on the identification plate is specified in the main chapter “General Information”, chapter “Device Identification”.

3.1.4 Mains Connection and Device Fuses

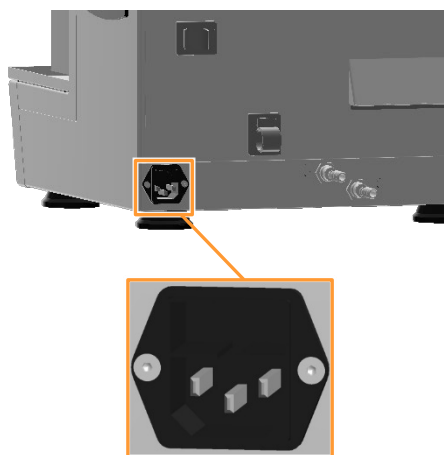


The mains connection is located on the rear side of the basic unit. The device is protected against excessive current consumption by two fuses. The device fuses are located directly above the mains connection.

The country-specific power cable required for connection to the power supply is included in the scope of delivery. If the power cable is defective, replace it with a power cable of the same type.

Before connecting the device, make sure that the voltage values of the device correspond to the local mains voltage. The mains connection must always be easily accessible so that the device can be disconnected from the power supply quickly in case of an emergency.

3.1.5 Water Connections

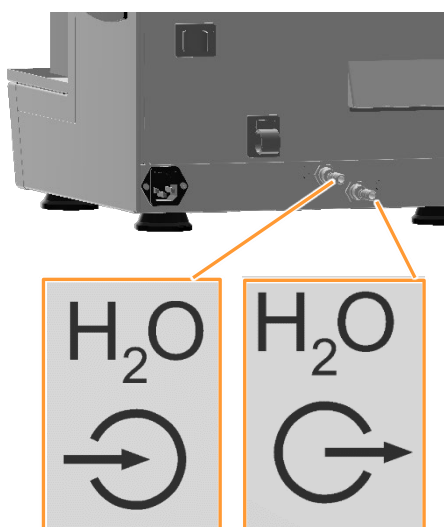


The two hose nozzles for connection of water inlet and outlet of the basic unit are situated on the rear side at the bottom of the basic unit. They are labelled with corresponding symbols:

- Left: Water inlet
- Right: Water outlet

Setup and Function


3.1.6 Gas Connections

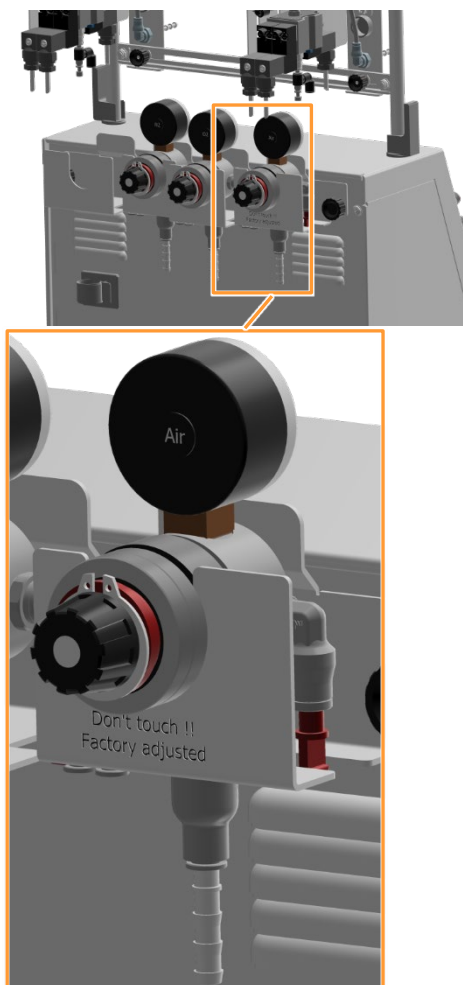

The gas connections are located at the top rear of the basic unit and are labelled with the corresponding gas. Each gas connection has a check valve, manometer and pressure reducing valve. The number of connections varies depending on the configuration.


The factory settings of a pressure reducing valve must not be changed!

Setup and Function

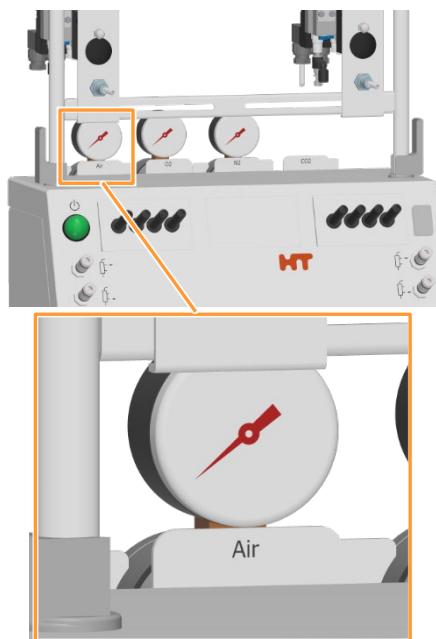

On the front of the device, the manometers are also clearly labelled with the corresponding gas.

3.1.7 Gassing Connection (Sparger)

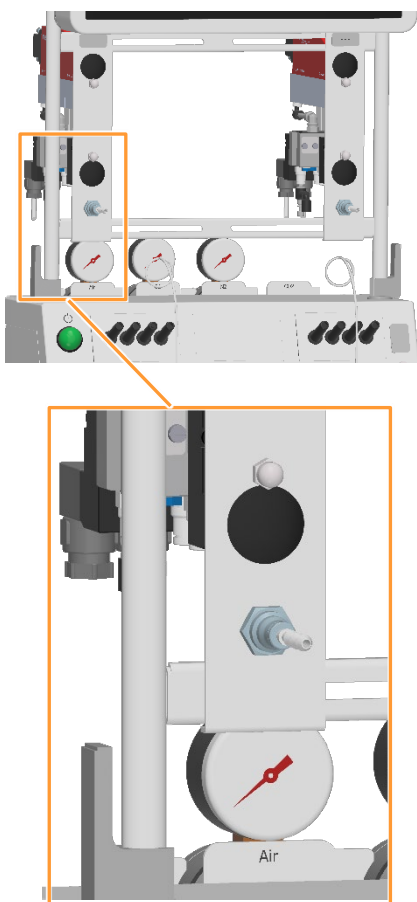

The hose nozzles for connection of the gassing hoses (sparger) are located on the front side of the gassing unit(s) ¹⁾.


i INFORMATION

Depending on the configuration and gassing strategy, hose lines must be merged by the operator using one or several Y-pieces.

¹⁾ Depending on the chosen gassing strategy, this can be rotameter(s), mass flow controller(s), solenoid valve(s).

Setup and Function

3.1.8 Sensor Connections (Sensor Cables)

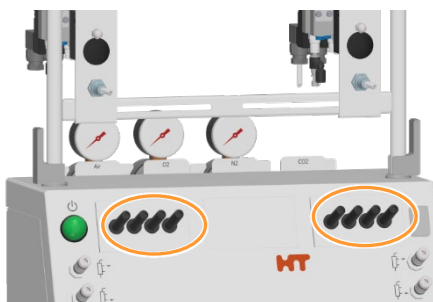


The basic unit is equipped and configured by default for measurement of temperature, pH, pO₂ and for foam detection ("antifoam"). This means, the temperature sensor (Pt100) and the cables for connecting the pH, pO₂ and antifoam sensor are always present. The appropriate antifoam sensors are included in the standard package, pH and pO₂ sensors are separately available.



INFORMATION


Depending on the chosen variant, the measurement system for pH and pO₂ is equipped and configured either for analog or digital sensors from the manufacturer METTLER or digital sensors from the manufacturer HAMILTON.

3.1.9 Connections Exit Gas Cooler and Valves for Water Flow

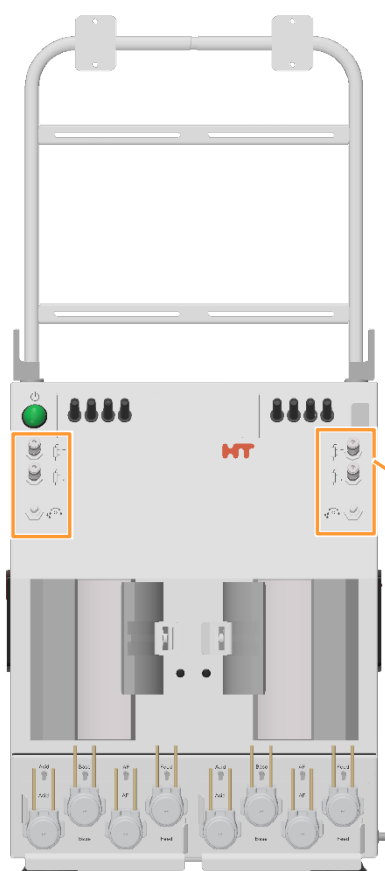

The water connections for the exit gas cooler and the manual valve for the water flow regulation are located on the left and right front side of the basic unit. The connectors are closed with plugs and the valves are covered with caps on delivery. The valves are factory adjusted. If needed, water flow can be manually adjusted here. Counter nuts are provided to lock the valves in their desired position.


Connections and valves are labelled with symbols (from top to bottom):

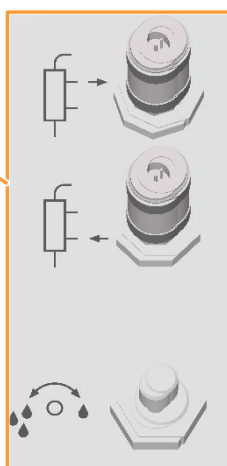

- Water outlet exit gas cooler
- Water inlet exit gas cooler
- Water flow regulation

Setup and Function


3.2 Operating Panel

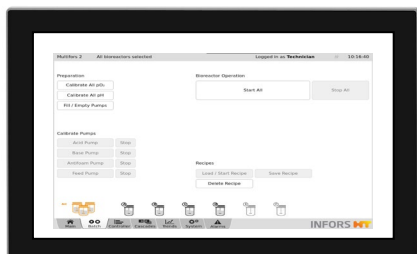

The operating panel is mounted on the device frame of the basic unit using a vertically swiveling bracket. It has a 15.6" color touch screen with protection type IP66. The operating panel is switched on using the power switch.

Up to six bioreactors (= culture vessels) can be individually or in parallel controlled by one operating panel.

A detailed description of the touch screen software can be found in the separate manual.

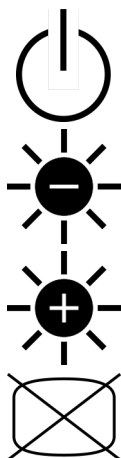

Monitor Keys

ON/OFF key

DECREASE brightness key: to set the display illumination darker

INCREASE brightness key: to set the display illumination brighter

DISPLAY key: to switch the display on/off

Special details about the ON/OFF key

The touch screen operating panel is switched on and off at the power switch on the basic unit. Therefore, separate switching on at the **ON/OFF** key is not necessary. The symbol on the key is illuminated when the operating panel is switched on.

Switching the operating panel off during a running process is the equivalent to a power failure!


Operating Panel Connections

Four connections are labeled and are used as follows:

- **LAN:** Ethernet
- **COM:** display cable
- **USB2.0:** for backups and service purposes
- **DCin:** power supply cable

Two additional connections are unlabeled and must not be used.

3.3 Culture Vessel

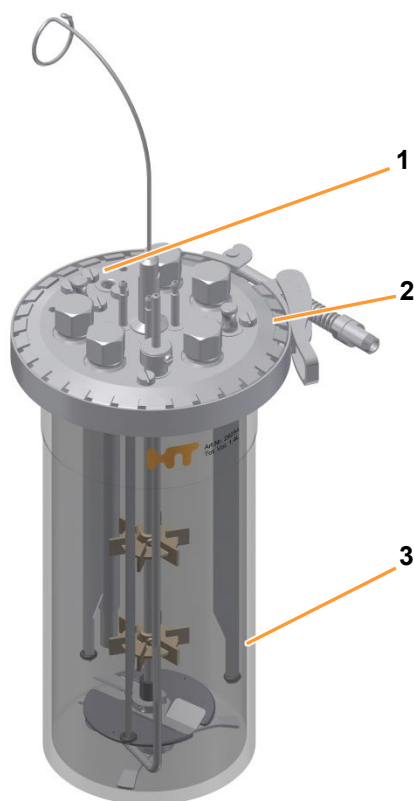


The culture vessel consists of the glass vessel and the vessel top plate with standard equipment and a clamping ring with quick-release fastener. The vessel is made of borosilicate glass and has a flat bottom.

- 1 Vessel top plate
- 2 Clamping ring with quick-release fastener
- 3 Glass vessel

The figure on the left shows a culture vessel with 1400 mL total volume. Three vessel sizes are available:

- 400 mL total volume / DN 70 / 55
- 750 mL total volume / DN 70
- 1400 mL total volume / DN 90

All culture vessels (2 per basic unit) are supplied in a vessel holder. The 400 mL culture vessel has an additional adapter for the thermal block. For details on vessel holder and vessel adapter see main chapter "Accessories".

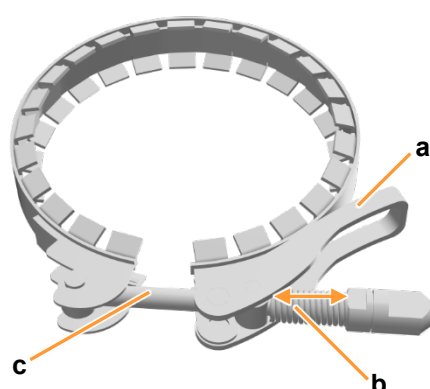


Clamping ring with quick-release fastener

The vessel top plate is held in place on the glass vessel with a clamping ring with quick-release fastener (a). To ensure sealing between the top plate and the vessel, the length of the spring (b) on the threaded rod (c) must be set correctly. Ex-factory, this length is set to 21 mm when the clamp is closed and must not be changed.

- Opening the clamping ring: Flip open the quick-release fastener and unhook the threaded rod.
- Closing the clamping ring: Hook in the threaded rod and close the quick-release fastener.

Setup and Function

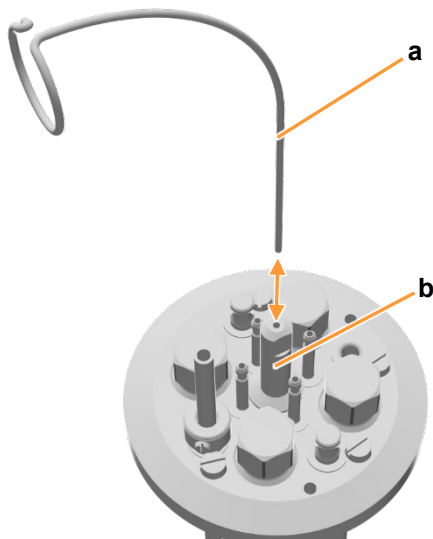


Hose Holder

The two-part hose holder for the hoses of the reagent bottles is located in the centre of the vessel top plate. The upper part, the piece of wire (a), is inserted into the opening of the lower part (b) that is screwed tight. This part is screwed to the bearing holder in the vessel top plate and is also used to hold in place the addition port adapters.

3.3.1 Ports in the Vessel Top Plate and their Configuration

The vessel top plate has different ports of different sizes to mount the different components such as sparger, blanking plugs, sensors etc. The number of ports in the top plate and its configuration depends on the nominal diameter (DN) = inner diameter) of the culture vessel.


3.3.1.1 Vessel Top Plate, DN 70/55

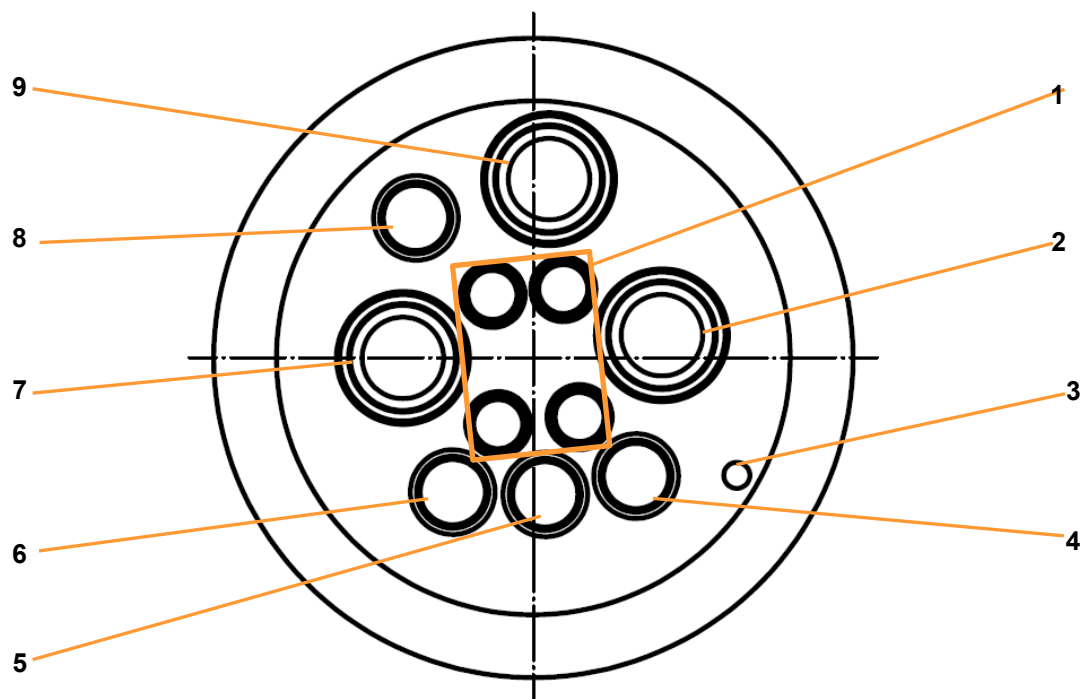

- | | | | |
|---|--|---|-----------------------------------|
| 1 | Ø 7.5 mm: addition port adapter, 4 pieces | 6 | Ø 10 mm: dip tube for sampling |
| 2 | Ø 12 mm / Pg13.5: pO ₂ sensor | 7 | Ø 12 mm / Pg 13.5: pH sensor |
| 3 | Ground connection antifoam sensor | 8 | Ø 10 mm: sparger |
| 4 | Ø 10 mm: antifoam sensor | 9 | Ø 12 mm / Pg13.5: exit gas cooler |
| 5 | Ø 10 mm: immersion pocket temperature sensor (Pt100) | | |


Setup and Function

3.3.1.2 Vessel Top Plate, DN 70

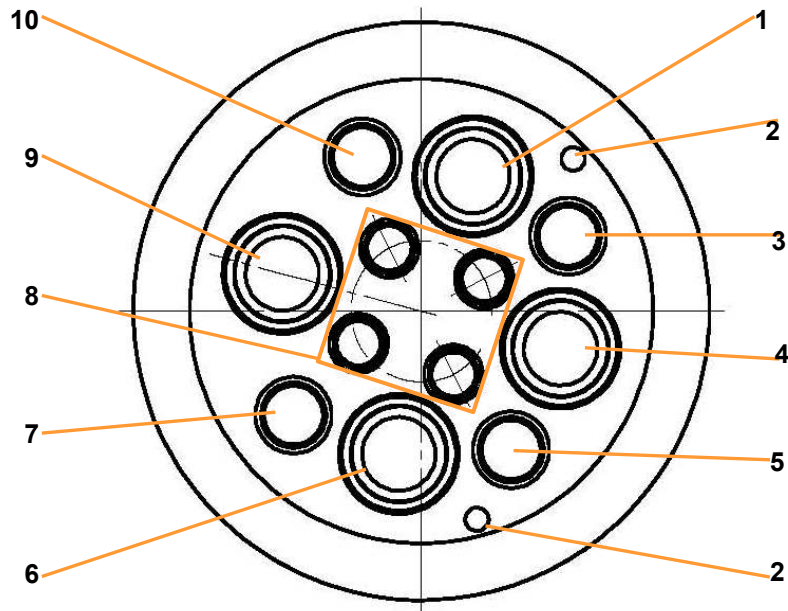

- | | | | |
|---|--|----|--|
| 1 | 12 mm / Pg13.5: pO ₂ sensor | 7 | Ø 10 mm: immersion pocket temperature sensor (Pt100) |
| 2 | Ground connection antifoam sensor | 8 | Ø 7.5 mm: addition port adapter, 4 pieces |
| 3 | Ø 10 mm: antifoam sensor | 9 | Ø 12 / Pg13.5 mm: exit gas cooler |
| 4 | 12 / Pg13.5 mm: pH sensor | 10 | Ø 10 mm: sparger |
| 5 | Ø 10 mm: dip tube for sampling | | |
| 6 | Ø 12 / Pg13.5 mm: inoculation | | |


3.3.1.3 Vessel Top Plate, DN 90

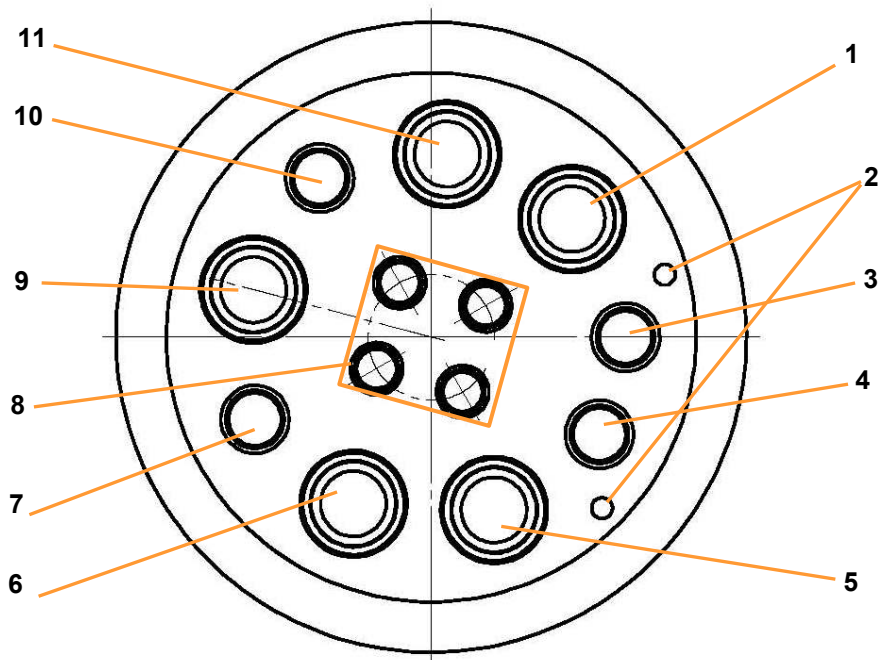

- | | | | |
|---|-----------------------------------|----|--|
| 1 | Ø 12 / Pg13.5 mm: pH sensor | 7 | Ø 10 mm: immersion pocket temperature sensor (Pt100) |
| 2 | Ground connection antifoam sensor | 8 | Ø 7.5 mm: addition port adapter, 4 pieces |
| 3 | Ø 10 mm: antifoam sensor | 9 | Ø 12 / Pg13.5 mm: exit gas cooler |
| 4 | Ø 10 mm: dip tube for sampling | 10 | Ø 10 mm: sparger |
| 5 | Ø 12 / Pg13.5 mm: spare | 11 | Ø 12 / Pg13.5 mm: pO ₂ sensor |
| 6 | Ø 12 / Pg13.5 mm: inoculation | | |

Setup and Function

3.4 Temperature Control System

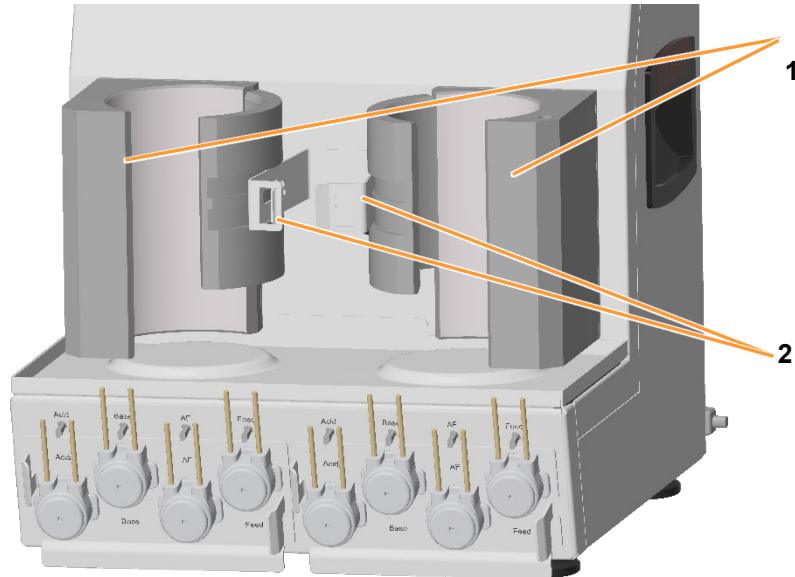

- 1 Thermal block
- 2 Clamp (snap closure)


The temperature control (heating and cooling) happens via two thermal blocks. The temperature in the culture vessels is measured with platinum resistance thermometers (Pt100 sensor). The temperature is transmitted from the thermal blocks to the culture vessels by means of heat exchange.

The thermal blocks are heated electrically by heating cartridges. Water flows through the thermal blocks for cooling.

A snap closure, consisting of two clamps, in the middle of the two thermal blocks fixes the culture vessels in the thermal blocks on the basic unit.

3.5 Stirrer

The stirrer shaft is activated from below via a DC external rotor motor. Power transfer between the motor shaft and the stirrer shaft is contact-less and uses magnets. Depending on the vessel size, there are two or four magnets on the stirrer shaft and, as the counterpart, the same number of magnets on the motor shaft in the basic unit. The stirrer shaft turns counter-clockwise (vessel top view).

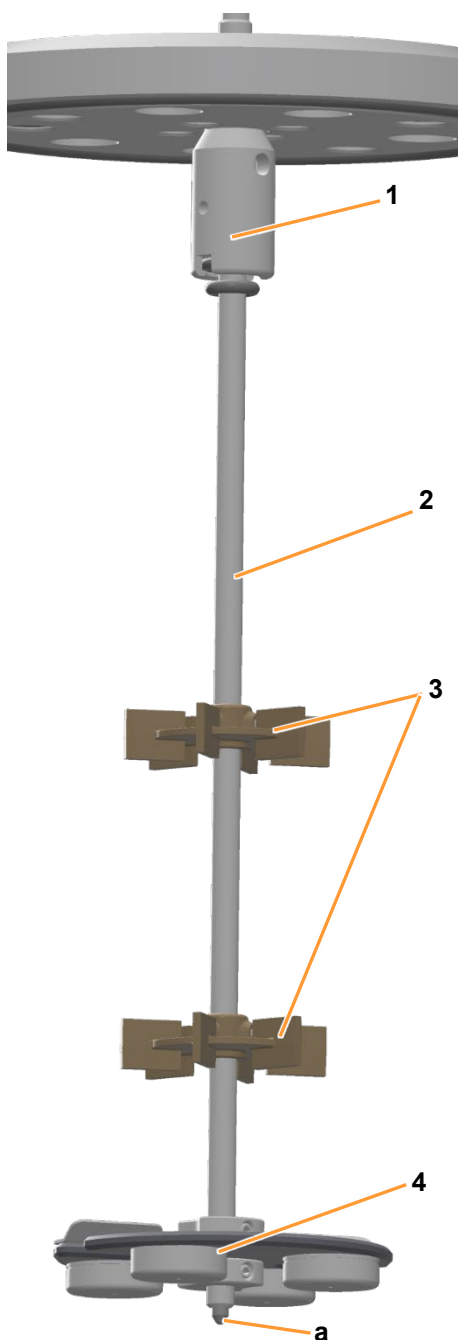


- 1 Bearing holder
- 2 Stirrer shaft with ceramic tip (a)
- 3 Impeller
- 4 Magnetic coupling

The stirrer shaft has a bearing on each end. The upper bearing is located in the bearing holder in the vessel top plate and is held in place and sealed using O-rings. At the end of the stirrer shaft, there is a ceramic tip (a). This is inserted into a centering bearing on the vessel bottom and holds the stirrer shaft in place there.

Setup and Function


Centering bearing

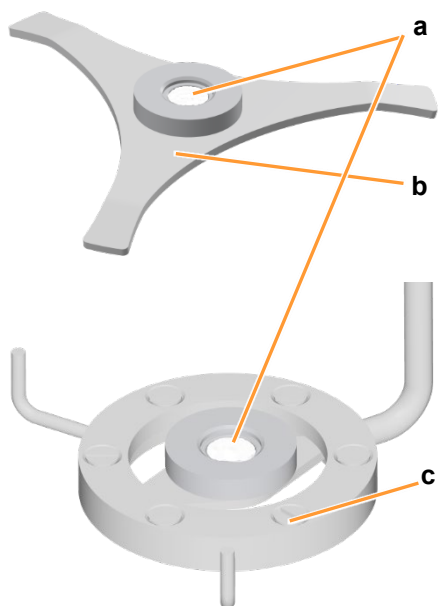

- With 400 mL and 1400 mL vessels, the centering bearing (a) is anchored in a triangular plate (b).
- With 750 mL vessels, the centering bearing (a) is anchored in the centre of the aeriation ring (c) of the sparger.

Magnetic coupling and flow deflector

The figures show the flow deflector (a) and the magnetic coupling with magnet holder (b) and two strong magnets (c).


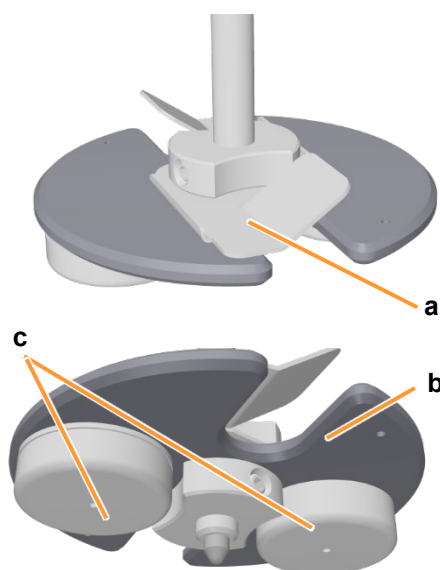


! ATTENTION

Danger of material damage caused by magnetic fields. Magnetic fields can damage laptops, hard drives, ATM cards, data media and other items susceptible to magnetism.

- Magnet holders in 400 mL and 750 mL vessels are equipped with two magnets.
- Magnet holders in 1400 mL vessels are equipped with four magnets.

Setup and Function

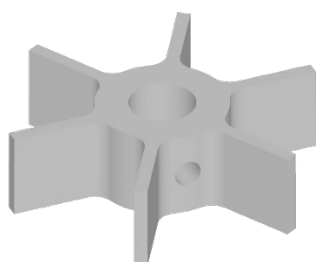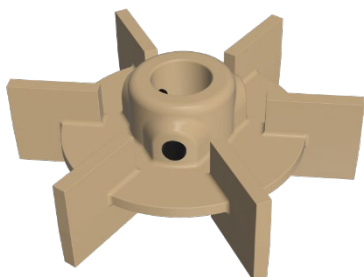

Impeller

By default, two Rushton impellers with 6 blades are used. The impellers are made from Peek and are attached to the stirrer shaft with two grub screws.



INFORMATION

Exception: for 400 mL vessels, two 6-bladed impellers (90°) made of 316L stainless steel are used, which are affixed to the stirrer shaft with a grub screw.

3.6 Gassing System

The basic unit is equipped with the appropriate gassing units (rotameter, solenoid valves, mass flow controllers and configured according to the chosen gassing strategy.

The following gases can be used:

- Air
- Oxygen (O₂)
- Nitrogen (N₂)

Optionally, carbon dioxide (CO₂) can be used instead of liquid acid for pH control.

Setup and Function

Gassing Strategy

The following variants are available:

Strategy	Description
"Basic"	■ Manual flow control via rotameter ■ Gasmix via solenoid valves
"Standard"	■ Flow control via one electronic mass flow controller. ■ Gasmix via solenoid valves
"High End"	■ Flow control and Gasmix via electronic mass flow controllers, 1 piece per gas

Additionally available is CO₂ sparger gassing for pH control. Addition and gas flow control takes place via electronic mass flow controller.

Gasmix System

The gas mixture takes place before entry into the culture vessel. The composition of the gas mixture is set and controlled in the touch screen software.

A detailed description of the touch screen software can be found in the separate operating manual.

Gas Entry

The gas or the gas mixture is led via a silicone hose from the gassing connection on the basic unit via sparger directly into the medium in the culture vessel. For details about the sparger see the main chapter "Accessories", chapter „Sparger“.

3.7 Exit Gas

Even without active gassing, any cultivation can increase the pressure inside the vessel through heating or gas production. As such, an exit gas line is essential for all cultivation processes.

Siphoning off exit gas via the exit gas cooler

The exit gas cooler dries the exit gas through condensation, thus preventing the exit gas filter from becoming clogged with moisture. At the same time, it also prevents liquid loss in the culture medium.

Setup and Function



INFORMATION

If heavy foaming is expected, a bottle of antifoam agent can be installed upstream of the exit gas filter as a foam trap.

The exit gas cooler is included in the standard package; for more details, see main chapter “Accessories”, chapter “Exit Gas Cooler”.

3.8 pH Control

The pH value in the medium is measured by the pH sensor and controlled by addition of reagents (acid, base) or by CO₂ gassing instead of using liquid acid. Addition of acid and base takes place via the two digital peristaltic pumps *Acid* and *Base*.

Reagent bottles are filled with acid and base which are connected to an addition port adapter in the vessel top plate and the two pumps by silicone hoses.

CO₂ led via sparger into the culture medium. It is added via electronic mass flow controller, see also chapter “Gassing Strategy”.

Measurement system

Depending on the variant selected, the measurement system for pH is equipped and configured for analog or digital sensors manufactured by METTLER or digital sensors manufactured by HAMILTON.

Measurement system variants	Properties
METTLER analog	- Conventional pH sensor (potential measurement against reference) - Type: 405-DPAS-SC-K8S/120
METTLER digital	- Conventional pH sensor (potential measurement against reference) with built-in electronics - Type: InPro 3253i, ISM
HAMILTON digital	- Conventional pH sensor (potential measurement against reference) with built-in electronics - Type: Easyferm Plus ARC



INFORMATION

pH sensors type Easyferm Plus ARC are preconfigured by the device manufacturer INFORS HT. Replacement sensors must be configured before use!

Setup and Function

For details on the technical data, use, maintenance and storage of the pH sensors, see the separate documentation provided by the sensor manufacturer. Read and follow the instructions.

Calibration

As a general rule: Calibration of a pH sensor always must be carried out **BEFORE** autoclaving. This is executed on the touch screen operating panel. For details refer to the separate operating manual of the touch screen software.



INFORMATION

If the pH sensor has already been calibrated externally, the bio-reactor will use this data and there is no need for calibration on the operating panel. This only applies to digital pH sensors.

Mounting

pH sensors are mounted into a 12 mm / Pg13.5 port by the means of a sensor holder. For details see main chapter “Accessories”, chapter “Sensor Holder”.

3.9 pO₂ Control

The oxygen saturation of the (culture) medium is measured by the pO₂ sensor, and can be adjusted as follows:

Increasing the pO₂

The content of the oxygen dissolved in the medium (pO₂) can be increased using the following methods:

- Increasing the stirrer speed
- Increasing the gas volume flow rate (air and/or oxygen)
- Increasing the oxygen content in the Gasmix

These approaches can also be combined

pO₂ reduction

In anaerobic processes, the vessel can be gassed using nitrogen. This displaces the oxygen dissolved in the medium.

For details about pO₂ control refer to the separate operating manual of the touch screen software.

Setup and Function

Measurement system

Depending on the variant selected, the measurement system for pO₂ is equipped and configured for analog or digital sensors manufactured by METTLER or digital sensors manufactured by HAMILTON.

Measurement system variants	Properties
METTLER analog	■ Conventional, amperometric/polarographic pO₂ sensor ■ Type: InPro 6820
METTLER digital	■ pO₂ sensor with integrated opto-electronics ■ Type: InPro 3253i, ISM with choice of: - Classic, with Opto-Cap, straight - HD, with Opto-Cap angled, with "Anti-Bubble" technology low-noise measurement signal
HAMILTON digital	■ pO₂ sensor with integrated opto-electronics ■ Type: Visiferm RS485-ECS with choice of: - ODO Cap H3, standard applications - ODO Cap H4, convex, more robust

Polarisation

Polarographic pO₂ sensors must be polarised for initial operation or after they have been disconnected from the power source.



INFORMATION

Digital pO₂ sensors are preconfigured by the device manufacturer INFORS HT. Replacement sensors must be configured before use.

For details on the technical data, maintenance and storage of the pO₂ sensors, see the separate documentation provided by the sensor manufacturer. Read and follow the instructions.

Measurement and Calibration

Generally speaking, the following applies: Unlike measurements such as pH, which are calibrated to absolute measurement values, the oxygen measurement is always calibrated to a relative reference point. For this purpose, the calibration is set to 100 % relative oxygen saturation, usually with air at max. stirring speed and maximum gas flow rate. The absolute concentration of dissolved oxygen in mmol/L may therefore vary at 100 % saturation, depending on the process.

Setup and Function



INFORMATION

Depending on the specifications defined by the user, the pO₂ sensor will be calibrated either before the vessel is filled with medium or afterwards, in the prepared medium.

For details about calibration refer to the separate operating manual of the touch screen software.

Mounting

pO₂ sensors are mounted into a 12 mm / Pg13.5 port by the means of a sensor holder. For details see main chapter “Accessories”, chapter “Sensor Holder”.

Setup and Function


3.10 Antifoam Control

Foam hinders the exchange of gas between the medium and the gas phase in the head space. The exit gas filter can become clogged with foam, which causes a pressure build-up in the vessel. This can be prevented by adding antifoam agent.

The antifoam agent is kept in a reagent bottle that is connected to the antifoam sensor and the antifoam pump via a hose. The sensor also acts as a dosing needle. When the sensor comes in contact with foam, the antifoam pump is activated and antifoam agent is fed into the vessel via the dosing needle.

Antifoam Sensor

Inside diameter	2 mm
Hose connection outside diameter	4 mm

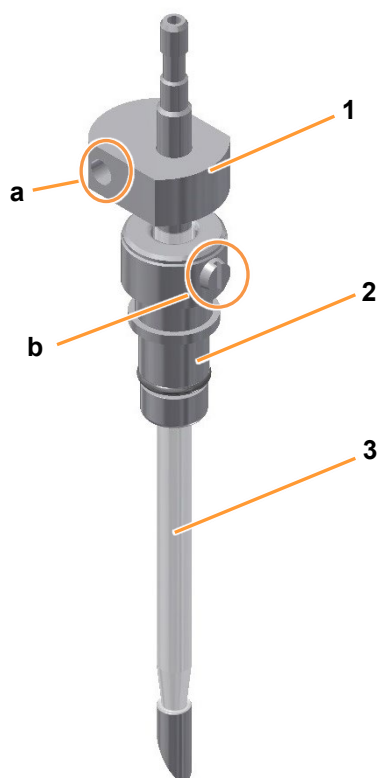

A clamping adapter with a O-ring is used to mount the sensor in the 10 mm port in the vessel top plate.

- 1 Sensor head with port for banana connector (a)
- 2 Clamping adapter with slotted-head screw (b)
- 3 Needle with transparent insulation

The antifoam sensor is equipped with two NON-autoclavable protective caps.

**INFORMATION**

A version of the antifoam sensor with an inner $\varnothing = 3$ mm for $\varnothing 12$ mm / Pg13.5 ports is also available with the appropriate clamping adapter. For details see main chapter "Accessories", chapter "Antifoam Sensor".

Options

4 Options

The following options are available in addition to the equipment included in the scope of supply for the basic unit.

4.1 Pump(s)

In addition to the four pumps available as standard, an additional analog peristaltic pump (*Feed 2*) can be integrated. As for the standard analog feed pump, its speed can be variably adjusted in steps of 0.1 % within a range from 0 % to 100 %.



External Pump(s)

One or more Watson Marlow 120U/DV external peristaltic pump(s) are also available. The number of possible external pumps depends on the options already available.

Like the other analog peristaltic pumps, the pump speed is adjustable and can be set in steps of 0.1 % within a range of 0 % to 100 %.

For further information on safety, use, maintenance and technical data of the pump(s), refer to the separate documentation of the pump manufacturer.

4.2 Balances

The touch screen software allows the connection of one balance to the bioreactor. If more than one balance is to be connected, the connection via the bioprocess software eve® is required.

Balances of the following type are available from the device manufacturer:

- Kern DS 30K0.1-A
- Kern FKB 6K0.02-B
- Mettler MA6002
- Mettler MA32001L

In addition to a specific device firmware, these balances also require a suitable configuration, which is carried out by the device manufacturer. This is the only way to ensure smooth functionality.

Non-configured and non-listed models are not supported.

If, however, a non-listed balance is to be integrated or several balances of a compatible type are to be used, there is the option of

integration into the eve bioprocess software®. Please contact the device manufacturer.

4.3 Level Detection

The level sensor detects liquid in the vessel. As soon as this happens, the measurement display shows “100”. This signal can be used as required for level control in the vessel in order to keep the working volume in the vessel constant. This can be done, for example, by using a simple cascade to control the feed pump or an optional pump that pumps liquid either into or out of the vessel. Special configurations are possible on request.

Level Sensor

The type of level sensor with clamping adapter without O-ring for mounting in a Ø 12 mm / Pg13.5 port in the vessel top plate is supplied as standard.



- 1 Connection for banana connector of sensor cable
- 2 Clamping adapter with slotted screw (A)
- 3 Sensor shaft with transparent insulation

The level sensor is equipped with two NON-autoclavable protective caps.

Level sensor types with clamping adapters for Ø 10 mm are available, too. For details about clamping adapters, refer to main chapter “Accessories”.

Options

4.4 Exit Gas Analysis

In order to allow the user to draw conclusions regarding the status of the culture while the bioprocess is still underway, the CO₂ and O₂ measurements are often taken and analyzed in the exit gas flow of the bioreactor.

4.4.1 Measurement Systems (Gas Sensors)

As measurement system for exit gas analysis are combined CO₂ and O₂ gas sensors of the type BlueInOne Ferm, BlueInOne Cell or BlueVary available.

Measurement ranges gas sensors

Type gas sensor	Vol. % CO ₂	Vol. % O ₂
BlueInOneFerm	0 to 10	1 to 50
	0 to 25	1 to 50
BlueInOneCell	0 to 10	0 to 100
BlueVary (cartridge ZrO ₂)	0 to 10	0.1 to 50
	0 to 25	0.1 to 50
BlueVary (cartridge eC)	0 to 10	0 to 100
	0 to 25	0 to 100
	0 to 25	0 to 25

For details on the safety, technical data, usage, and maintenance requirements for the gas sensors, see the separate documentation provided by the sensor manufacturer BlueSens. Read this documentation before using the gas sensor and follow the instructions contained therein.

4.4.2 Connecting the Gas Sensors

In order to view measurements on the operating panel, the measuring system for exit gas analysis must be connected to the bioreactor.

The gas sensor must be connected to the sensor cable and the bioreactor's exit gas must be led into the sensor via hose line. Generally, the cable connection is established only once during installation and remains then. The connection to the exit gas line must be re-established before each cultivation process.

The ideal connection conditions are detailed in the separate documentation provided by the manufacturer.

Connecting the sensor cable

The fixed sensor cable is pre-installed in the factory (rear of device). The cable has an 8-pin round plug connector. In order to connect the sensor, the plug connector is plugged into the socket marked Port **A** on the gas sensor.

Due to the length of the sensor cable, the gas sensor can be positioned in a large number of possible locations.

Establishing the hose connection

3 m of pressure hose, D = 8 x 14.5, and a hose clamp are provided with the device in order to establish the hose connection between gas sensor and culture vessel (exit gas filter).

The hose connection between the culture vessel (exit gas filter) and the gas sensor must be designed in line with the direction in which the gas flows through the gas sensor.

Proceed as follows:

Procedure

1. Cut as short a piece as possible off the supplied pressure hose.
2. Push one end of the hose onto the hose nozzle (observe direction of flow) on the gas sensor's flow adapter and fasten in place with the clamp.
3. Push the open end of the hose onto the exit gas filter on the exit gas cooler.

**INFORMATION**

Do NOT use a clamp here, as the hose must be easy to disconnect at this point, e.g. for autoclaving the culture vessel.

4.4.3 Calibration

1-point calibration must be carried out once per month and after installation in order to guarantee exact measurement results.

This is done directly on the gas sensor itself. The procedure is described in the separate documentation provided by BlueSens.

4.4.4 Replacing the BlueVary Gas Sensor Cartridge

The max. operating time of a BlueVary gas sensor cartridge amounts to 9000 operating hours. Once this limit is reached, measurement is no longer possible. I.e. there is no measurement value output anymore and the display turns red. The gas sensor cartridge must be replaced by the sensor manufacturer.

Options

4.5 Multiplexer (Gas Switching Module)

To be able to measure exit gas values - usually O₂ and CO₂ - while bio processes are running in parallel, every single bioreactor usually has to be equipped with the corresponding measurement system (see chapter “Exit Gas Analysis”). Using one or more of the device's manufacturer's Multiplexers makes it possible to use only a single measurement system for this. The exit gases from the individual bioreactors are directed sequentially to the measurement system used by means of the gas switching module(s). The determined values are assigned to the corresponding bioreactor.

When using Multiplexers, the measurement information for the individual culture vessels is not available continually since one measurement sensor sequentially measures the exit gas of all culture vessels. The measurement interval achievable for each culture vessel depends, among other things, on the gas volume stream and the hose type used as well as its length.

4.6 Turbidity Measurement

Turbidity measurement can be used to draw conclusions regarding the biomass concentration in the culture. To determine the turbidity in the culture two measuring systems are available:

Variant ASD12-N

Technical specifications		
Sensor (Single channel light absorption) with integrated transmitter		
Sensor type	ASD12-N	
Selection of optical path lengths	OPL01	for very high cell densities
	OPL05	for higher cell densities
	OPL10	for lower cell densities
Absorption measurement range	0 to 4 CU	

The ASD12-N sensors supply a non-linearised turbidity measurement for the culture. This can be linearised manually using the soft sensor in eve®, for example, in order to determine correlation with factors such as the biomass concentration or optical density.

**INFORMATION**

If the temperature of the sensor rises above 50 °C during operation in the medium, an automatic switch-off takes place. After the medium has cooled down, the measurement continues automatically.

Variant CGQ BioR**Technical specifications**

Sensor (non-invasive scattered light measurement) with transmitter integrated in the basic equipment (CGQ BioR gateway)

Sensor type	CGQ BioR with two LEDs / measurement modes	
Selection of Mess-modi (LEDs)	Green: (521 nm)	for low cell densities
	Infrared: (940 nm)	for high cell densities
Measurement range	0 to 1000	

**CAUTION**

The light emitted by the LEDs on the sensor plate is highly sensitive and can damage the iris or retina. The CGQ BioR sensor plate contains an infrared LED that emits high energy radiation in the invisible range. Sensor plates with this LED carry the warning symbol shown on the left.

- Wear safety goggles and never expose eyes or skin to radiation without protection!
- Always keep a safety distance of >1 m from active sensor plates.
- Pause or stop running measurements before all work within the safety distance.

**INFORMATION**

CGQ BioR sensors are optimised for microbial bioprocesses. The sensors may be used in temperatures from 15 to 50 °C.

The CGQ BioR sensors non-invasively measure the scattered light of the culture. This is proportional to the biomass concentration in the bioreactor, but can also be processed, e.g. by a soft sensor in eve®, in order to obtain a correlation with the optical density.

Details and specifications of the sensors and their measuring principles as well as safety, use and maintenance can be found in the

Options

separate documentation of the manufacturers. Read these before using the turbidity sensor and follow the instructions.

4.6.1 Calibrating the Sensor

Variant ASD12-N

ASD12-N sensors are pre-calibrated ex-factory. Inserts are available for reference measurement.

Due to the different light absorption of different media, zero point calibration should be performed before each cultivation process. This can be done on the operating panel, either **before or after** autoclaving, depending on the application in question. For more details, refer to the separate operating manual of the touch screen software.

Variant CGQ BioR

CGQ BioR sensors are pre-calibrated ex-factory. A new calibration is not necessary.

4.6.2 Mounting the Sensor

Variant ASD12-N

The sensors can be mounted directly into 12 mm/Pg13.5 ports. An additional adapter is necessary for mounting into a 19 mm port. To adjust the mounting depth, a sensor holder is required for mounting. For more details on the sensor holder, refer to main chapter "Accessories" chapter "Sensor Holder".

Note the following points for mounting:

- Ensure that the sensor is fitted with an O-ring; fit an O-ring if necessary.
- Mount the sensor by hand – do not use any tools!
- If the mounting depth of the sensor is adjustable (mounting with sensor holder), make sure the mounting depth is set correctly prior to autoclaving, as later adjustment represents a contamination risk.
- Mount the sensor in such a way that it cannot come in contact with other components or the glass vessel.
- Mount the sensor in such a way that it has good access to the flow and there is no risk of bubbles collecting in the measurement gap.

Variant CGQ BioR

CGQ BioR sensors are always attached to the culture vessel with the strap attached to the sensor. For this purpose, the sensor with

Options

the measuring window is pressed against the glass vessel and fixed with the strap. Depending on the culture vessel, different positions of the sensor or attaching methods may be necessary. For mounting details, see separate documentation of the sensor manufacturer.

Note the following points for mounting:

- Ensure that the sensor is not attached to markings or stickers on the glass vessel, this may affect the measurement.
- Mount the sensor so that it is not in front of or in the direct vicinity of reflective steel parts (< 20 mm).
- Ensure that the sensor is positioned in such a way that liquid is in front of the measurement window during the entire bioprocess
- Foam, high gas hold-ups and the use of antifoam agents can (significantly) interfere with the light scattering of growing cells.

4.6.3 Interferences Turbidity Measurement

Interference		
Displayed measured value is not plausible / unusual		
Possible Cause	Remedy	By
Sensor cable is twisted or kinked or not properly connected.	Check and ensure that the sensor cable is not kinked or twisted. Connect the sensor cable properly as necessary.	Operator
ASD12-N: sensor is not calibrated	Calibrate the zero point	Operator
ASD12-N: window fouling on the sapphire windows.	Carefully clean the sensor	Operator
CGQ BioR: sensor is mounted in the wrong place / measures in foam	Place the sensor at the level of the liquid. Make sure that there are no obstacles in front of the measuring window.	Operator
Faulty sensor cable	Replace sensor cable	INFOR HT service technician
Faulty sensor cable	Replace the sensor	Operator

Options

4.7 Permissive Measurement

Sensors of the ABER Futura systems measure the permittivity (also: *capacitance*) and conductivity of the culture. This measured data can be used to determine a correlation with the live biomass concentration, for example, using the soft sensor in eve® or data evaluation.

The sensor with the corresponding transmitters must be purchased directly from the manufacturer ABER. INFORS HT offers a connection to the transmitter on the basic unit.

Measured parameters	Value	Unit
Permittivity	0 to 400	pF cm ⁻¹ range
Conductivity	0 to 40	mS cm ⁻¹ range

Calibration is performed according to the manufacturer's guidelines directly on the transmitter.

All information about the ABER Futura system is available in the separate documentation provided by the manufacturer.

4.8 Redox Measurement

The reduction/oxidation potential (redox) in the medium is measured using the redox sensor.

Measurement system	Properties
HAMILTON digital	■ Classic combined sensor (oxidation reduction potential measurement against a reference) with integrated electronics ■ Type: Easyferm Plus ORP ARC ■ Measurement range: -1500 mV to +1500 mV

The redox sensor can be connected instead of the HAMILTON pO₂ sensor. If the sensor is configured in addition to the HAMILTON pO₂ sensor, or if the system is configured for METTLER sensors, an additional connecting cable is required.

Calibration

Calibration is possible with a corresponding redox buffer solution using a HAMILTON Arc Handheld or a HAMILTON Arc USB cable. Both of these are available separately from the sensor manufacturer.

For details on the technical data, usage and maintenance requirements for the redox sensors, see the separate documentation of the redox sensor.

Mounting of the sensor

Redox sensors (both variants) are mounted into a 12 mm / Pg13.5 port in the vessel top plate by the means of a sensor holder. An additional adapter is necessary for mounting the sensor into a 19 mm port. For details about the sensor holder see main chapter "Accessories", chapter "Sensor Holder".

4.9 Conductivity Measurement

A sensor with a construction based on the 4-electrode principle is used to measure the conductivity in the medium. This ensures excellent linearity in the measurement range from 1 to 300000 $\mu\text{S}/\text{cm}$. The transmitter is integrated in the sensor head.

Technical specifications

Sensor, type	Conducell 4USF ARC with built-in electronics
Measurement range	1 $\mu\text{S}/\text{cm}$ to 300'000 $\mu\text{S}/\text{cm}$
Accuracy	$\pm 3 \%$ at 1 to 100000 $\mu\text{S}/\text{cm}$ $\pm 5 \%$ at 100000 to 300000 $\mu\text{S}/\text{cm}$
Manufacturer sensor	HAMILTON



INFORMATION

Conductivity sensors are preconfigured by the device manufacturer INFORS HT. Replacement sensors must be configured before use!

Calibration

The conductivity sensors are pre-calibrated ex-factory. They have a self-diagnosis function which, among other things, also outputs calibration recommendations. In order to be able to use this function, the corresponding software or hardware must be obtained directly from the sensor manufacturer.

For details about technical data, use and maintenance of the conductivity sensor, refer to the separate documentation from the sensor manufacturer.

Options

Mounting of the sensor

Conductivity sensors are mounted into a 12 mm / Pg13.5 port in the vessel top plate by the means of a sensor holder. For details about the sensor holder see the main chapter “Accessories”, chapter “Sensor Holder”.

Accessories

5 Accessories

The table below lists all the accessories included in the standard package, divided according to nominal diameter (= inside diameter) and vessel size (TV = total volume). Since each device features two culture vessels, all item numbers are specified x 2, with the exception of the vessel holder and starter set.

Accessories	DN 70 / 55	DN 70	DN 90
	TV 400 mL	TV 750 mL	TV 1400 mL
Ring sparger, Ø 4 mm	1 x 2	--	1 x 2
Ring sparger, Ø 4 mm, with aeration ring	--	1 x 2	--
Rushton impeller, PEEK	--	2 x 2	2 x 2
Blade impeller, 6 blades (90°), 316L	2 x 2	--	--
Immersion pocket for temperature sensor in port Ø 10 mm	1 x 2	1 x 2	1 x 2
Baffles	--	--	1 x 2
Blanking plug for port Ø 7.5 mm	2 x 2	2 x 2	2 x 2
Blanking plug for port Ø 10 mm	2 x 2	2 x 2	2 x 2
Blanking plug for port Ø 12 mm/Pg13.5	4 x 2	3 x 2	5 x 2
Addition port adapter Ø = 4 x 2 mm for port Ø 7.5	4 x 2	4 x 2	4 x 2
Septum collar for port Ø 12 mm / Pg13.5	1 x 2	1 x 2	1 x 2
Clamping adapter for port Ø 10 mm / with inside Ø 6 mm	2 x 2	1 x 2	1 x 2
Clamping adapter for port Ø 10 mm / with inside Ø 4	1 x 2	2 x 2	2 x 2
Dip tube Ø 4 mm (for sampling system)	1 x 2	1 x 2	1 x 2
Vessel adapter DN 70/55 for culture vessel	1 x 2	--	--
Adapter sleeve for port 12 mm Pg13.5 for exit gas cooler	1 x 2	--	--
Super Safe Sampler sampling system for port Ø 10 mm (with clamping adapter and dip tube, also listed separately)	1 x 2	1 x 2	1 x 2
Antifoam sensor for port Ø 10 mm (with clamping adapter with inside Ø 6 mm, listed separately)	1 x 2	1 x 2	1 x 2
Vessel holder	1	1	1
Exit gas cooler	1 x 2	1 x 2	1 x 2
Reagent bottle, 250 mL 3+1 connections	4 x 1	4 x 1	4 x 1
Starter set	1	1	1




INFORMATION

The following chapters describe the standard accessories supplied with the device and optional accessories, too.

Accessories

5.1 Vessel Holder

The height-adjustable vessel holder is used to attach the culture vessel to the basic unit and also acts as a carrying frame.

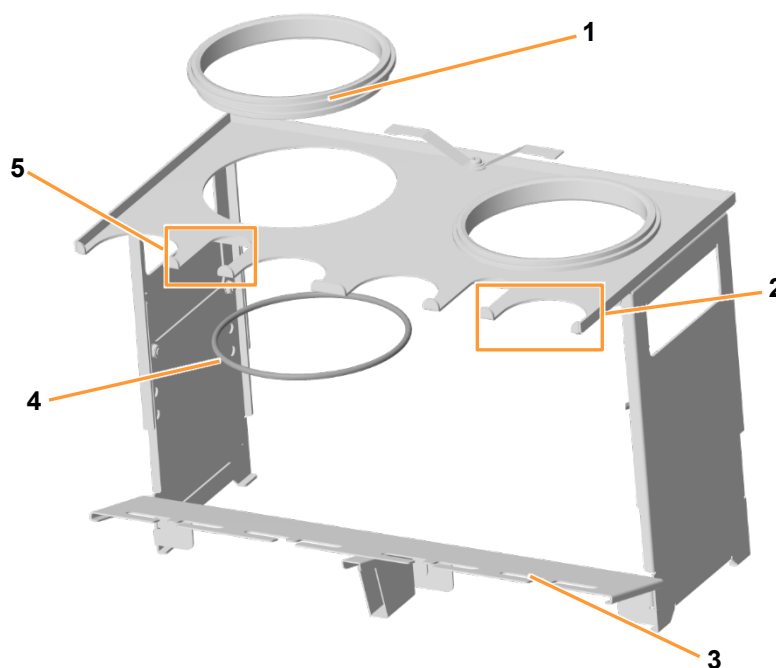


- 1 Centering ring (2 pieces)
- 2 Holder for reagent bottle (4 x)
- 3 Holder for mounting plates with pump heads (2 x)
- 4 O-ring (2 pieces)
- 5 Holder for reagent bottle (2 x)

To ensure the culture vessels fit exactly, centering rings with the corresponding nominal width and suitable O-rings are inserted into the holder so that the vessel flange sits flush.


The frame has holders for hanging up four reagent bottles and two smaller laboratory bottles. Holders for inserting two mounting plates with four pump heads each are also available.

The culture vessels can thus be transported to the autoclave together with the reagent bottles and pump heads and be sterilized as one unit.

Accessories

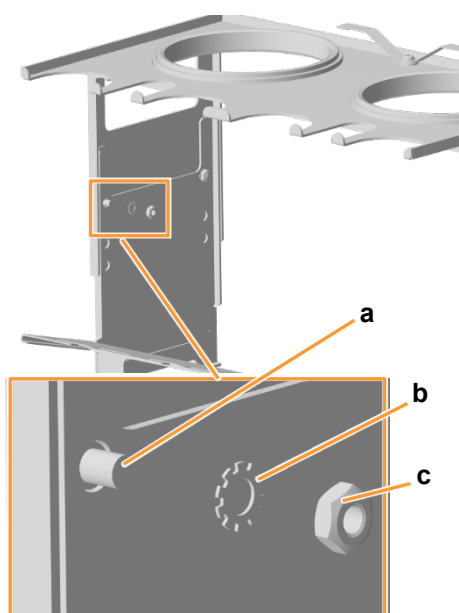

The side walls of the vessel holder consist of two parts, allowing the upper part equipped with a bolt (a) to be adjusted in height. The lower part has recesses at three different heights. It is fastened with a serrated washer (b) and hexagon nut M4 (c) on each side.

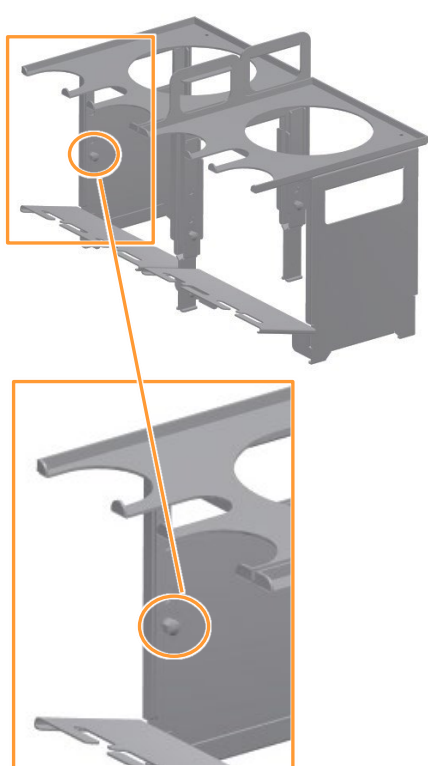


Two individual, interlocking frames are also available. These are fastened using two serrated washers and cap nuts M4 on each side wall.

Accessories

5.2 Vessel Adapter

The vessel adapter is included with 400 mL culture vessels, because their vessel flange has a larger nominal diameter (70 mm) than the vessel body (55 mm). The vessel adapter is required for fitting into the thermal block on the basic unit.

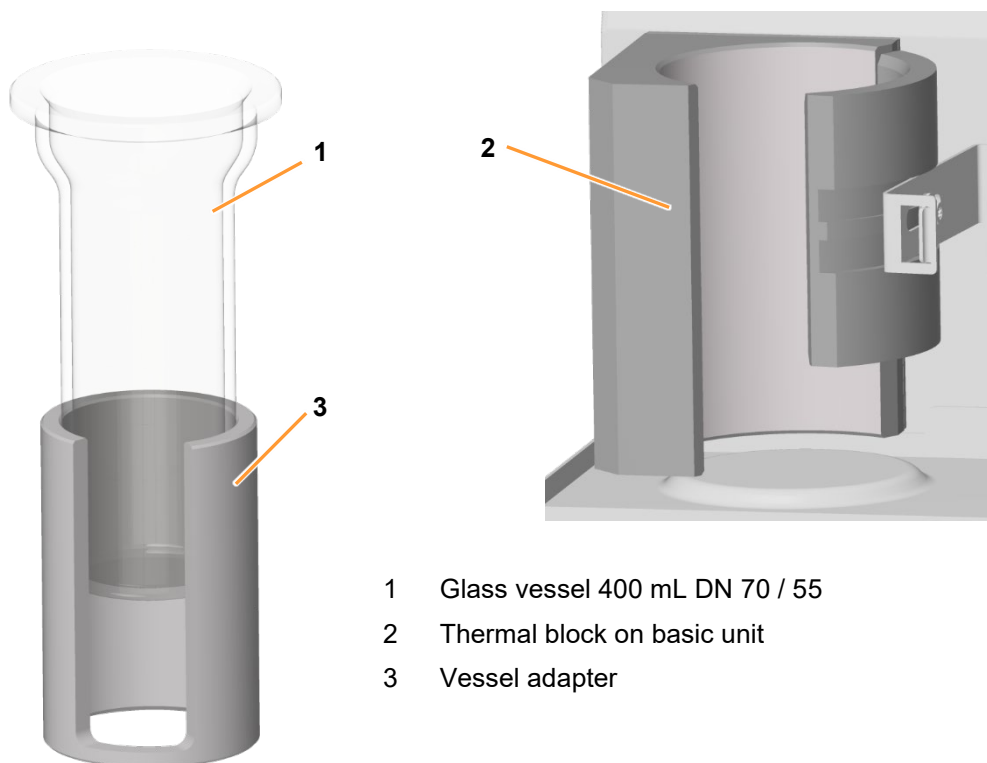

5.3 Sampling System Super Safe Sampler

Basically different systems and also individual components are available for sampling. This operating manual describes the operation and handling of the aseptic sampling system Super Safe Sampler combined with a dip tube.

The use of the Super Safe Sampler prevents the culture vessel from contamination when sampling.


Content of the set

The set consists of a completely pre-assembled group of valves with hoses and two syringes. It is connected via silicone hose with a dip tube.




Valve assembly

- 1 Sterile filter
- 2 Check valve
- 3 Luer activated sample valve
- 4 T-piece
- 5 Hose

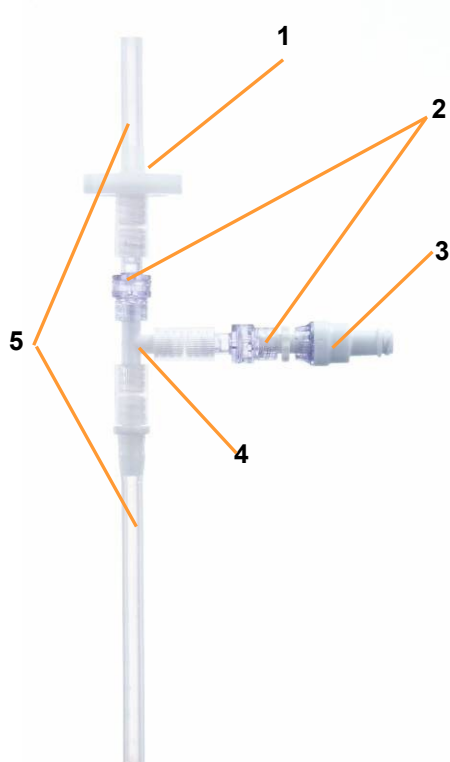

The valve assembly consists of a T-piece, two check valves, a Luer-activated automatic sample valve, a sterile filter, a length of hose as an adapter for the syringe and another hose for connection to the sample dip tube in the culture vessel.

Accessories

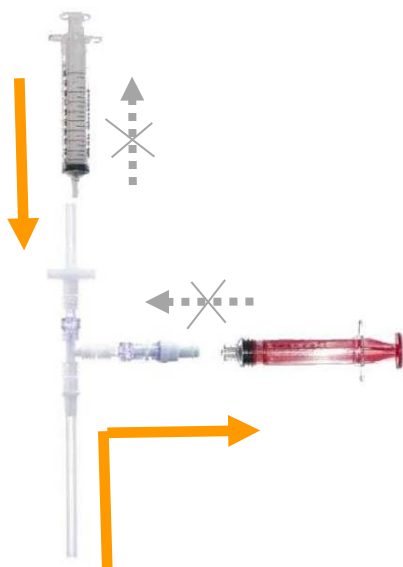

Principle of function

The sample valve on the side arm of the T-piece opens by putting the Luer connector of the syringe into the valve and closes by removing the syringe. No further handling is necessary.

Unintentional re-introduction of the sample material once it has been withdrawn is prevented by a check valve. Thus, contamination of the bulk culture is impossible.

Following sampling, a second syringe can be fitted and air pushed in via the sterile filter, in order to displace culture solution from the sample hose and the dip tube of the vessel. With a conventional sampling system, the next sample cannot be taken immediately, as rinsing of the sampling hose and the immersion tube is necessary. By previously removing most of the culture in the sampling line, this sampling system can save culture volume, which is particularly important with small vessels and/or frequent sampling.

The dead volume of the culture remaining in the group of valves after flushing with sterile air amounts to a few μl and is negligibly small. If the withdrawal of a very small sample volume is required, with minimum possibility of falsification, a small quantity of culture solution (e.g. 1 ml) can be introduced and rejected before the actual sample is taken.

Designated use

The Super Safe Sampler is designed for aseptic sampling of completely liquid samples.

Solid parts in the sample may lead to clogging of the valves. Therefore, employing the Super Safe Sampler for solid media is not recommended.

The Super Safe Sampler is autoclavable (not the syringes!) and for this reason reusable.

Practical tips for the use of the Super Safe Sampler

Sterility of the culture vessel is ensured at all times without the possible measures mentioned below.

The use of a sterile syringe and sterile caps is only necessary if the sample has to be processed under sterile conditions. For sampling, the same non-sterile syringe can be used repeatedly, without fear of contamination of the culture vessel.

Aseptic Sampling

For each sample, use a new, sterile syringe with Luer Lock fitting, in order to ensure the sterility of the sample.

Sterile syringes are consumables and therefore not included in the set.



INFORMATION

The use of another syringe is also possible. But a syringe with Luer lock prevents unwanted movement of the syringe.

- Before fitting the syringe, disinfect the sample valve. For this, spray a commercially available disinfectant onto the valve.
- After spraying and after each sampling, close the the sample valve with a sterile Luer-Lock cap (Dead End Cap) to keep the valve and sample sterile.

The caps are not included in the kit. Very convenient to use are so-called combi-caps that fit on male and female connectors alike.

Caps that are vented and made of steam sterilizable material can also be fitted during autoclaving.

Accessories

5.4 Sparger

The gas is fed directly into the medium via a sparger by default. The sparger is mounted in a 10 mm port in the vessel top plate using a clamping adapter, and connected to the gassing system on the basic unit via a silicone hose with a sterile filter.

Ring sparger

Inside Ø	4.0 mm
Outside-Ø hose connection	6.0 mm



Sparger with aeration ring

Inside Ø	4.0 mm
Outside-Ø hose connection	6.0 mm
Use	750 mL culture vessel

This sparger has an aeration ring on its lower end. The centering bearing of the drive shaft (not visible in the figure to the left) sits the middle of the aeration ring.

**5.5 Impellers**

For details about impellers, refer to chapter “Setup and Function”, “Stirrer”.

5.6 Immersion Pocket for Temperature Sensor (Pt100)


The immersion pocket is a pipe with a sealed bottom end, and is used to insert the temperature sensor.

Immersion pocket Ø 10 mm

Fitted with O-ring.


One or two slotted screws (a) are used for fixation in the 10 mm port, depending on the vessel size.

The illustration on the left does not show the full length of the immersion pocket.

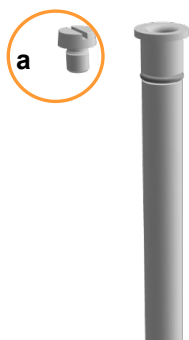


Accessories


5.7 Baffles

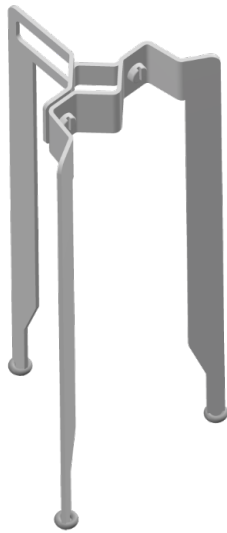

1400 ml culture vessels are equipped as standard with a two-part baffle cage with three baffles. The baffles are equipped with O-rings.

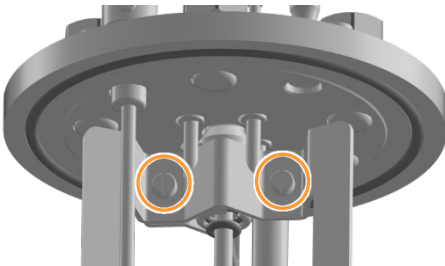

The baffles are fixed to the bearing holder. Two slotted cheese head screws are used for mounting.

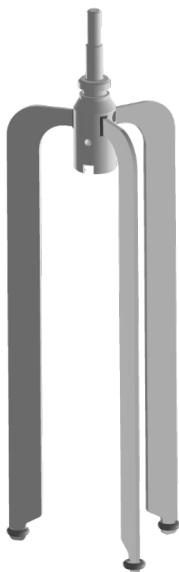

For 750 ml culture vessels, the three baffles are as one-piece available, which is firmly welded to the bearing holder.


5.8 Blanking Plugs

Blanking plugs are used to seal open ports. There are different blanking plugs for the different types of port.

Blanking plug, Ø 10 mm

Fitted with O-ring.

Depending on the vessel size, one or two slotted screw(s) is/are used for fixing in the 10 mm port.

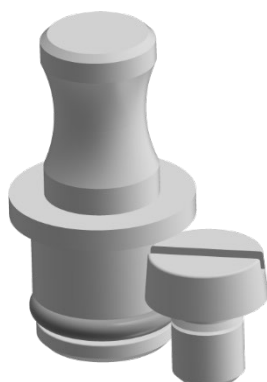

Blanking plug, Ø 12 mm

Must be fitted with an O-ring before being mounted in the 12 mm/Pg13.5 port.

Mounted using a thread.



Blanking plug, Ø 7.5 mm


Fitted with O-ring.

The reagent bottle hose holder is used for fixing in the 7.5 mm port (same principle as for the addition port adapters).



Accessories

5.9 Addition Port Adapters

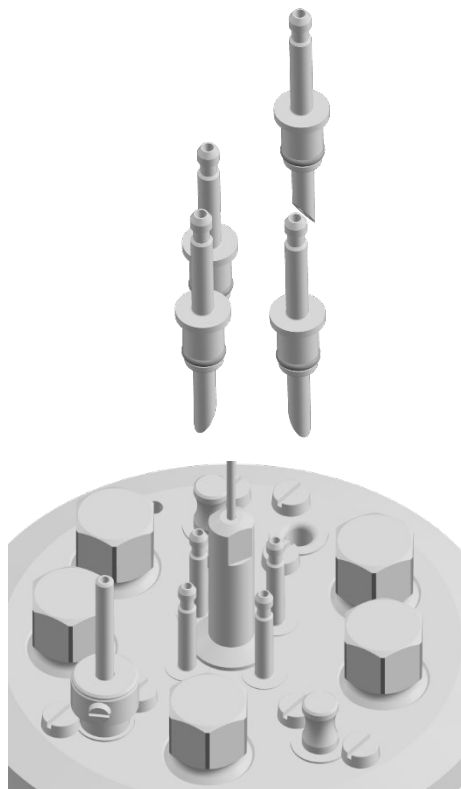

The four addition port adapters are used for liquid addition into the culture vessel and end in the headspace of the vessel. They have a hose connection, are equipped with O-rings and are mounted into the four 7.5 mm ports in the vessel top plate. The addition port adapters have an oblique tip and their long sides face outwards in mounted state.

The reagent bottle hose holder is used for fixing the four addition port adapters in their ports.

Inside-Ø	2 mm
Outside-Ø hose connection	4 mm
Mounting depth	17 mm

The following can be connected to addition port adapters:

- Reagent bottles
- If appropriate, exit gas line
- If appropriate, gassing hose for headspace gassing

5.10 Inoculation Needles

Inoculation needles are used for feeding liquids into the culture vessel, which cannot be autoclaved with the culture vessel. These liquids may be e.g. the inoculum or heat-sensitive reagents.

If using an inoculation needle, then a septum (inoculation membrane) must be fitted along with a septum collar in the appropriate port. The inoculation needle is connected with the reagent bottle and autoclaved. The liquid, e.g. the inoculum, which shall to be added into the culture vessel, is shortly before addition filled into the reagent bottle under sterile condition. The septum is then pierced with the inoculation needle, which is screwed into the septum collar. The septum may be wetted e.g. with an alcohol solution that is lit up before the piercing.

Accessories

Inoculation needles are purchased including septum collar. They have an oblique tip to facilitate the piercing. The hose connection and the very sharp needle tip are covered with non-autoclavable(!) protective caps.



INFORMATION

The piercing method with inoculation needle is rather unsuitable for vessel sizes of the device described in this operating manual. But inoculation needles can be used without septum collar and without septum like addition port adapters or dip tubes for addition of autoclavable liquids.

Inoculation needle Ø 12 mm

Inside-Ø	2.5 mm
Outside-Ø hose connection	4.5 mm

Must be fitted with O-ring.

Thread is used for mounting in septum collar for a 12 mm / Pg13.5 port.



5.11 Septum Collars

Septum collars are either used in combination with the corresponding inoculation needle with septum or with a syringe with injection needle and a septum. Inoculation needles are always supplied including a septum collar, but septum collars are separately available, too.

Accessories



Septum collar, Ø 12 mm

With internal thread.

A septum must be inserted in the 12 mm / Pg13.5 port before mounting.

A thread is used for mounting.

5.12 Dip Tubes

Dip tubes are open at both ends and are mounted in a vessel top plate port with a clamping adapter.

Dip tubes are used for a variety of purposes:

- For filling the culture vessel after autoclaving. Using a dip tube prevents foaming.
- For adding inoculum.
- For sampling. The aseptic Super Safe Sampler system can be used for sampling.
- For harvesting
- For siphoning off medium during continuous cultivation
- For draining the culture vessel

Depending on the purpose, silicone hoses are connected to the dip tube via other vessels, sampling systems or, if necessary, hose trees.

Multiple dip tubes can be used at any one time, providing that enough vessel top plate ports are available.

Different types of dip tubes are available.

Accessories**Dip tube, straight Ø 4 mm**

Inside-Ø	2.0 mm
Hose connection outside-Ø	4.0 mm

The dip tube does not reach to the vessel bottom.
The illustration on the left shows only the upper section of the dip tube.

Dip tube, straight, Ø 6 mm

Inside-Ø	3.0 mm
Hose connection outside-Ø	5.0 mm

The dip tube does not reach to the vessel bottom.
The illustration on the left shows only the upper section of the dip tube.

Accessories



Dip tube, slightly curved, Ø 6 mm

Inside-Ø	4.0 mm
Hose connection outside-Ø	6.0 mm

The dip tube does (nearly) reach to the vessel bottom.

5.13 Clamping Adapters


Clamping adapters are used for mounting the sparger, the various dip tubes and the antifoam/level sensors. The clamping adapter fixes the component part in place and can be used to adjust its mounting depth.

The clamping adapter must match the outside diameter of the part to be mounted and the size of the port.

Clamping adapter Ø 4 mm / 10 mm

Fitted with O-ring (B).

Depending on the vessel size, one or two slotted screw(s) is/are used for fixing in the 10 mm port.

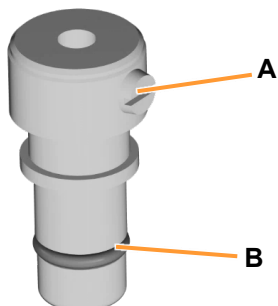


After loosening the slotted screw (A) the component part with Ø 4 mm can be inserted into/pulled out from the clamping adapter. The component part is fixed in the clamping adapter by fastening the slotted screw.

Clamping adapter Ø 6 mm / 10 mm

Fitted with O-ring (B).

Depending on the vessel size, one or two slotted screw(s) is/are used for fixing in the 10 mm port.

After loosening the slotted screw (A) the component part with Ø 6 mm can be inserted into/pulled out from the clamping adapter. The component part is fixed in the clamping adapter by fastening the slotted screw.

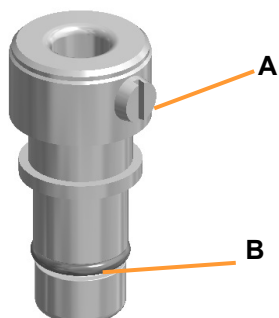


Clamping adapter Ø 6 mm / 12 mm

Must be fitted with O-ring before mounting.

Thread is used for mounting in 12 mm / Pg13.5 Port.


After loosening the slotted screw (A) the built-in part with Ø 6 mm can be inserted into/pulled out from the clamping adapter. The built-in part is fixed in the clamping adapter by fastening the slotted screw.

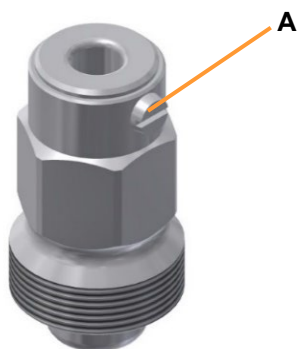

5.14 Sensor Holder

Sensor holders are used to adjust the mounting depth of sensors (pH, pO₂, etc.) in 12 mm/Pg 13.5 ports. The sensor holder, respectively the sensor must be fitted with an O-ring for mounting.

The sensor holder comprises a sheath with a grub screw, a guide bar with a fork, and a hollow screw. The wrench for the grub screw is also included in the scope of supply.

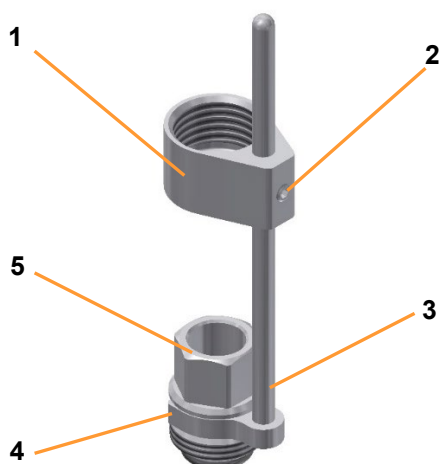


- 1 Sheath
- 2 Grub screw
- 3 Guide bar
- 4 Fork
- 5 Hollow screw

Accessories

5.15 Exit Gas Cooler


The exit gas cooler dries the exit gas through condensation, thus preventing the exit gas filter from becoming clogged with moisture. At the same time, it also prevents liquid loss in the culture medium. The exit gas is passed through the cooling pipe of the exit gas cooler. The cooling is done by water, which is led through the jacket of the cooling pipe. A baffle in the cooling pipe serves to extend the residence time of the exit gas in the cooling pipe. The water supply to the exit gas cooler is provided by the basic unit. The water flow rate can be adjusted using the manual valve on the basic unit.

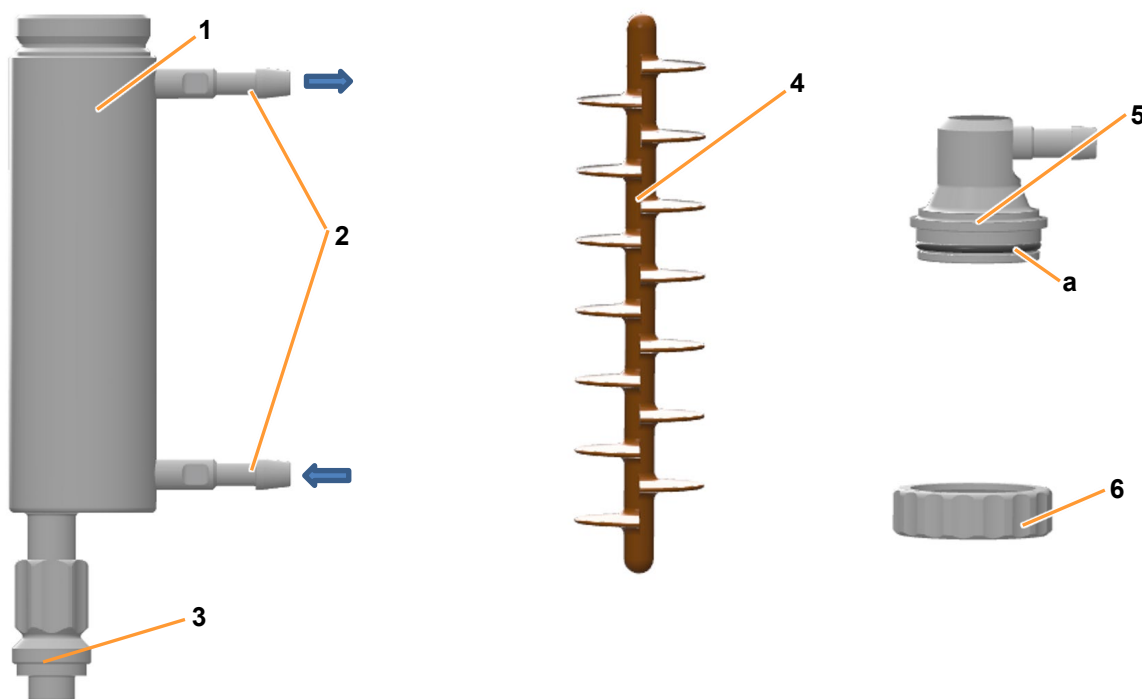

- | | | | |
|---|---|---|---------------------|
| 1 | Cooling pipe with jacket | 4 | Baffle (silicone) |
| 2 | Hose connections water inlet (lower) and water outlet (upper) | 5 | Lid with O-ring (a) |
| 3 | Screw thread | 6 | Coupling nut |

Accessories

The exit gas cooler is supplied pre-fitted with a piece of pressure hose an exit gas filter and pressure hoses for water inlet (lower connector) and water outlet (upper connector). Hoses and filter are secured with hose clamps.

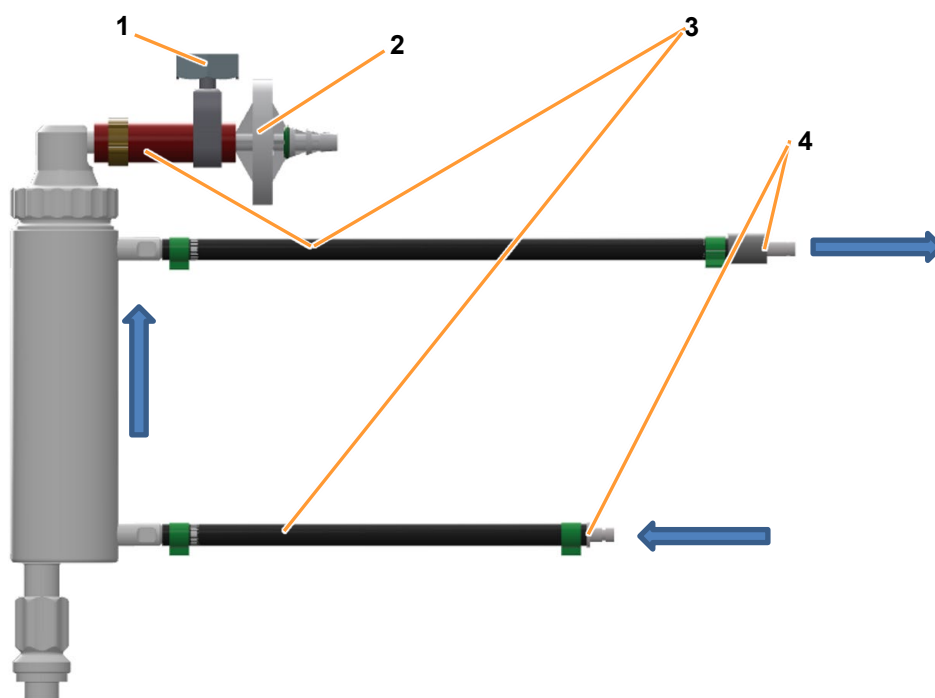

- 1 Adjustable hose clamp
- 2 Exit gas filter

- 3 Pressure hose
- 4 Rapid coupling with plug-in nozzle

Important notes


- The exit gas cooler only works when the temperature control system is switched on.
- The exit gas filter must be replaced with a new filter after each cultivation process.

Mounting


The exit gas cooler must be equipped with an O-ring before mounting. Its thread is used for mounting it into the 12 mm / Pg13.5 port.

Accessories

5.16 Adapter Sleeve

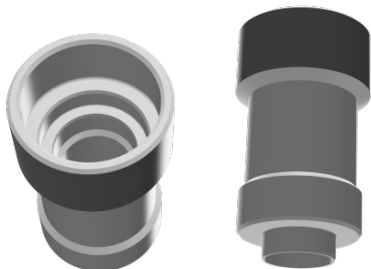

The adapter sleeve is used for mounting the exit gas cooler into the 12 mm / Pg13.5 port in the vessel top plate of the 400 mL culture vessel to facilitate manipulation of other built-in parts.

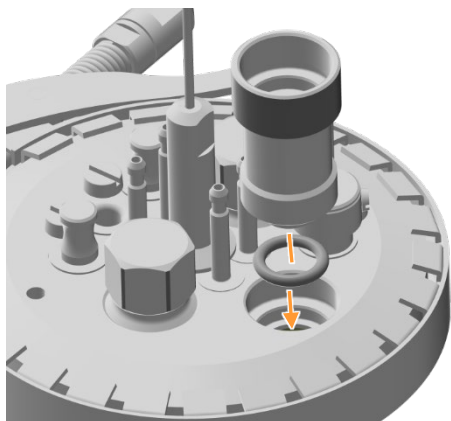


The adapter sleeve must be equipped with an O-ring before mounting into the 12 mm / Pg13.5 port. The exit gas cooler, which is also fitted with an O-ring, can then be screwed into the adapter sleeve.

5.17 Reagent Bottles

For addition of corrective reagent and feed solution (substrate) into reagent bottles with made of borosilicate glass 3 + 1 or 2 hose connections are available.

Size	Ø Hose	Number of hose nozzles
250 mL	2 x 6 mm	3 + 1 (Standard)
250 mL	2 x 6 mm	2

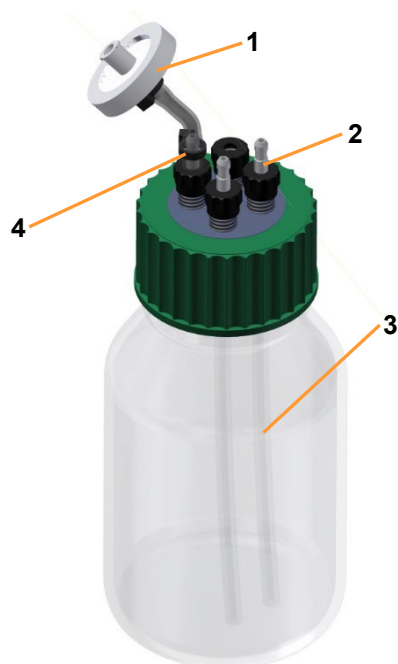Accessories

By default, reagent bottles with 3 + 1 hose connections are supplied. A reagent bottle is connected to two culture vessels (two bioreactors = 1 basic unit).

The reagent bottles are supplied equipped with:

- 1 Filter
- 2 Hose connection (hose nozzle)
- 3 Silicone hose
- 4 Cable tie

Three of the four connections are provided with hose nozzles. Two hose nozzles are fitted with silicone hoses at the lower end and on the inside of the lid. The silicone hoses provided in the starter set for connection to the culture vessels are connected to the same hose nozzles on the outside of the lid.

The third hose nozzle is equipped with a silicone hose and a filter for pressure equalization. The filter is secured with cable ties.

The fourth connection on the reagent bottle is closed with a silicone stopper. As a spare a fourth hose nozzle is separately in the bottle set.



The picture to the left shows the reagent bottle type with 2 hose connectors.

Accessories

5.18 Antifoam Sensor


In the standard package of the device, the antifoam sensor is supplied in the version for a Ø 10 mm port in the vessel top plate. For details see main chapter “Setup and Function”, chapter “Anti-foam Sensor”.

A version of the antifoam sensor with matching clamping adapter for Ø 12 mm / Pg13.5 ports is available separately.



Length	Inside-Ø	Hose connection outside-Ø
250 mm	3 mm	4 mm

5.19 Pump Heads

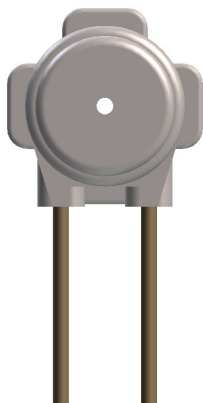

The autoclavable pump heads are fitted with PharMed pump hoses prior to delivery. Three different hose diameters are available for different delivery rates:

- 1.0 mm (standard)
- 0.5 mm
- 2.5 mm

For more detailed information about pumps and hoses refer to main chapter “Technical Data”, chapter “Specifications”, “Pumps”.

5.20 Sterile Filters

Sterile filters are used to protect against contamination in both the gassing line and the exit gas line. In addition to this, all reagent bottles used for pressure equalization must be fitted with a short piece of hose with a filter.

All the sterile filters in the scope of supply are autoclavable, disposable filters with PTFE diaphragms.



INFORMATION


Sterile filters must be clean and dry at all times, and should thus ideally be replaced after each use.

Ø 37 mm, marked red




Application	Supply air
Retention rate	0.2 µm

Accessories




Ø 37 mm, marked green

Application	Exit gas
Retention rate	0.3 µm dry 1.0 µm wet



Ø 25 mm, not marked

Application	Super Safe Sampler
Retention rate	0.2 µm



Ø 25 mm, not marked

Application	Reagent bottles (pressure equalization)
Retention rate	0.45 µm
Diaphragm	PTFE

Accessories

5.21 O-Rings and Gaskets

Description	Ø mm	Utilisation
O-Ring,	1.5 x 5.0	Gasket, port size 7.5 mm
O-ring, EPDM	1.5 x 7.5	Gasket, port size 10 mm
O-ring, EPDM	2.62 x 10.77	Gasket, port size 12 mm / Pg13.5
O-ring, EPDM	3.50 x 82.14	Top plate gasket culture vessel DN 70/55 and DN 70 (set of 2 pieces)
O-ring, EPDM	3.50 x 101.19	Top plate gasket culture vessel DN 90 (set of 2 pieces)
O-Ring, EPDM	1.78 x 2.9	Stirrer shaft (upper part)
O-Ring, EPDM	2.4 x 3.3	Stirrer shaft (below bearing holder) and baffles, both models
O-Ring, EPDM	2.0 x 8.0	Bearing holder (2 pieces)
O-Ring, EPDM	1.5 x 3.5	Gasket, clamping adapter Ø 4
O-Ring, EPDM	1.78 x 528	Gasket, clamping adapter Ø 6 mm
Flat gasket, Silicone	32 x 42 x 2	Gasket for reagent bottle lid (model with two hose connections)
O-ring, EPDM	2.0 x 26	Lid gasket for exit gas cooler

5.22 Hoses and Hose Accessories

Hose type	Ø mm	Utilisation
Pressure hose, red, fibreglass-woven	8 x 14.5	Water supply and return basic unit
Pressure hose, red, fibreglass-woven	6 x 11.9	Gas connection, exit gas filter attachment (on exit gas cooler)
Pressure hose, transparent	4.0 x 8.0	Water supply and return, exit gas cooler
Silicone hose	4 x 7	Hose from gassing unit (e.g. rotameter, MFC) to inlet air filter and on Y-pieces
Silicone hose	3 x 6	Sparger hose to the inlet air filter
Silicone hose, transparent	2 x 6	Reagent bottles (hose lines for reagents)

Accessories

Hose Fitting	Ø mm	Utilisation
Hose clamp, screw with screwdriver slot, INOX	17	To fasten hoses for water supply and return to basic unit
Hose clamp, screw with hand cap, INOX	17	To fasten exit gas filter to hose piece on exit gas cooler
Hose clamp, screw with screwdriver slot, INOX	14	To fasten hose/hoses for gas connection
Screwless hose clamp	9 to 10	To fasten hoses for water supply and return to exit gas cooler
Screwless hose clamp	12.5 to 14	To fasten piece of pressure hose for exit gas filter
Hoffmann pinchcock, nickel-plated brass	12	To clamp off hose lines, e.g. on unused addition port adapters, clamping off the sparger hose, etc.
Cable tie, polyamide	2.4 x 85	Hoses for reagent bottles and pumps, inlet air filter, sparger, sampling system dip tube
Hose connector, 3/32" x 1/16", PVDF	---	To connect pump heads to hose with inside Ø 1 mm
Hose connector, 1/8" x 1/8", PVDF	---	To connect pump heads to hose with inside Ø 2.5 mm

5.23 Tools and Inoculation Accessories

Accessories for inoculation

Septum, Ø = 16 mm MVQ silicone, transparent, for 12 mm/Pg13.5 ports

Sterile disposable syringe, Luer, 10 mL, inside Ø 14.35 mm

Sterile hollow needle, 20G, L = 40 mm/Ø = 0.9 mm

Tool	Utilisation
Hexagon socket spanner SW17	Blanking plugs in 12 mm/Pg13.5 ports
Hex key SW1.27	Grub screws

6 Transport and Storage

The following specifications are based on transport and storage of an unpacked device at the provider's site.

6.1 Transport



WARNING

Improper transport, the use of incorrect auxiliary equipment and careless handling of the device may lead to injuries and severe property damage.

The following points must be observed when transporting the device internally (relocation):

- Always work in pairs and use suitable auxiliary equipment when transporting the device.
- The entire device (basic unit and culture vessel) contains delicate glass parts.
- Especially when using auxiliary tools, it is important to observe that the device's centre of gravity is not in the middle.



WARNING

The entire device (basic unit and culture vessel) is too heavy to be carried by one person alone.

Even the basic unit on its own exceeds the weight that should be carried by one person alone.

Transport and Storage

6.2 Storage

- Before each time they are put into storage, decontaminate, thoroughly clean and dry the culture vessel and all accessories ¹⁾.
- Store the device and its components clean, dry and protected against dust, dirt and liquids.
- Store the device and its components in a cool place with low air humidity but protected against frost.
 - Storage temperature: 5 °C to 55 °C
 - Relative air humidity, non-condensing: 10 % to 95 %.
- Protect the device from aggressive media, direct sunlight and mechanical vibrations.

¹⁾ *Maintain and store sensors produced by other manufacturers in accordance with the separate documentation.*

7 Installation and Commissioning

Installation and commissioning of the device may only be carried out by qualified personnel from the manufacturer or personnel authorised by the manufacturer.



WARNING

Installation and commissioning require qualified and experienced personnel. Faulty installation may lead to dangerous situations or severe loss of property.

Only let carry out installation and commissioning by the manufacturer's qualified personnel or authorised personnel by the manufacturer only.

Therefore, the following sections only list the energies that must be provided and the connection requirements that are to be respected on site by the provider.

Exception

The basic functions of the bioreactor are tested and demonstrated at the same time to the operator in form of a short test run on site during installation by the qualified personnel.

In order to become familiar with the basic functions of the bioreactor before the first cultivation or after a longer period of non-use of the device, the operator may afterwards carry out this short test run any time, too.

For details refer to chapter "Test Run".

7.1 General Location Requirements for Installation

The following requirements must be met for the installation of the device:

- The figures and ranges specified in the main chapter "Technical Data", chapters "Connection Values" and "Operating Conditions" must be observed.
- The device must only be installed inside a laboratory or a laboratory-like environment.
- The installation site must be level, sufficiently stable and able to bear loads.
- There must not be any sources of electrical interference near the device.

Installation and Commissioning

7.2 Minimum Distances

To operate and maintain the device it must be installed with a minimum spacing of 150 mm from walls, ceilings or other equipment.

7.3 Power Supply

The in-house electric power supply of the device must meet the following conditions:

- Single-phase, constant power supply
- Type 230 V / 50/60 Hz
- Type 115 V / 60 Hz

The power supply of the device must be made safe by the use of an FI-switch (or RCD – Residual Current Device) of the kind RCCB, Type B on the customer's side.

7.4 Water Supply and Return

The in-house water supply to the device, as well as the drainage of the water, must meet the following requirements

- “Very soft” or “soft” water quality (CaCO_3 concentration 0 mmol L^{-1} to 1.5 mmol L^{-1})



ATTENTION

Not observing the water quality requirements may lead to damage or failure of the device.

- Constant water supply at a pressure of 2 ± 1 bar
- Manometer to check the primary pressure available
- The drain is heat-resistant and without back pressure

Hoses

- Only use pressure-resistant and intact hoses.
- Only use appropriate hoses, use adapters as necessary.
- Secure hoses with the appropriate clamps.

Installation and Commissioning

7.5 Gas Supply

The in-house gas supply to the device must meet the following requirements:

- Constant gas supply at a pressure of 2 ± 0.5 bar
- Gas(es) is/are dry, clean and free of oil and dust
- Recommended compressed-air quality as per DIN ISO 8573-1: Class 1.2.1 for process air



ATTENTION

The use of impure gases can lead to blockage of the sterile filter and damage the mass flow controller.

Only use dry, clean and oil-free gases.

Hoses

- Only use pressure-resistant and intact hoses.
- Only use appropriate hoses, use adapters as necessary.
- Secure hoses with the appropriate clamps.



WARNING

The use of inappropriate or damaged hoses and/or inappropriate fixing may lead to leakage of gases. Depending on the gas in question, there may be a danger of gas explosion and/or danger of suffocation as well as a hazard for the health of the operator.

Always close the gas supply before a hose is removed and when the device is not in use.

7.6 Exit Gas

Ensure the following on the house side:

- The exit gas is safely discharged by means of a suitable, gas-tight hose.
- The working environment is equipped with an adequate ventilation system, depending on the application.

Installation and Commissioning

7.7 Test Run

In order to become familiar with the basic functions of the bioreactor before the first cultivation or after a longer period of non-use of the device, a short test run can be executed.

The test run comprises:

- Temperature control (cooling / heating)
- Stirring
- Gassing

Normal compressed air is used for gassing. To avoid calcium deposits, demineralised water is recommended for filling the vessel.

The following description of the test run does not detail handling of individual built-in parts, e.g. stirrer, sparger etc. Detailed descriptions of their handling are given in the corresponding chapters of the main chapter “Before Cultivation”.

For details on operation, refer to the separate operating manual of the touch screen software.

7.7.1 Preparation Test Run

Before starting the test run, check and ensure the following:

- All required services are available and activated.
- All services have the correct connection pressure.



INFORMATION

The following steps in the procedure refer to one bioreactor (= 1 culture vessel)

The following work is to be executed before the test run:

Procedure

1. Remove the vessel top plate and put it aside in such a way that it does not lie on top of built-in parts
2. Fill the culture vessel with water – preferably demineralised – to the working level.
3. Ensure that the stirrer and sparger are mounted; if necessary, mount them.
4. Fit the top plate and secure it by means of the clamping ring with quick-release fastener.

Installation and Commissioning

5. Screw the exit gas cooler into the port on the vessel top plate port.
The exit gas cooler is equipped with a new exit gas filter.
6. Connect the hoses of the exit gas cooler to the basic unit according to the symbols on the basic unit.
7. Close all remaining open ports with blanking plugs.
8. Connect the culture vessel in its holder to the basic unit and secure it with the snap closure.
9. Equip the sparger with a piece of silicone hose (D = 3 x 6 mm) for gassing and a dry, clean inlet air filter (accessories, filter with red label).
10. Fit another piece of silicone hose for gassing (D = 4 x 7 mm) to the hose nozzle for gassing (compressed air) on the basic unit.
11. Connect both hoses via the inlet air filter (connect the hose end to the hose nozzle of the inlet air filter).
12. Insert the temperature sensor as far as it will go into the immersion pocket in the top plate.



CAUTION

Risk of burns and loss of property due to elevated temperature!

The thermal block will overheat without an inserted temperature sensor and/or without liquid in the vessel. This can lead to burns and loss of property.

13. Switch the device on at the power switch and wait until the system is booted.

7.7.2 Cooling System

To activate the cooling system, proceed as follows:

Procedure

1. On the operating panel, set a low setpoint for the *Temperature* parameter, e.g. 10 °C, in order to activate the water supply to the temperature control system.
2. Start the bioreactor.
3. All parameters except for *Temperature* remain switched off; switch them off if necessary.
You should now hear water flowing into the temperature control system.
The water supply to the exit gas cooler should be activated, too now.
4. Use your hands to check whether the exit gas cooler and thermal block are beginning to cool down.

Installation and Commissioning

As soon as the temperature control circuit is full, water will flow out of the water outlet of the basic unit.

For the rest of the procedure, allow the bioreactor to run with temperature control switched on.

7.7.3 Stirring

Bioreactor is running with temperature control switched on

To test the stirrer, proceed as follows:

Procedure

1. On the operating panel for the parameter *Stirrer*, set a low setpoint.
For further information about the different ranges of rotation speed refer to the specification in main chapter “Technical Data”.
2. Switch the parameter on.

For the rest of the procedure, allow the bioreactor to run with the temperature control switched on and the stirrer running.

7.7.4 Heating and Adjusting Temperature

Bioreactor is running with temperature control switched on and stirrer running

To test the heating and adjust the temperature, proceed as follows:

Procedure

1. On the operating panel, set a high setpoint for the *Temperature* parameter, e.g. 45 °C.
The water supply for cooling is stopped; the system heats up.



CAUTION

Risk of minor burns if the heated thermal block is touched!

2. Wait until the temperature has adjusted to the setpoint.

For the rest of the procedure, allow the bioreactor to run with the temperature control switched on and the stirrer running.

Installation and Commissioning

7.7.5 Gassing

Bioreactor is running with temperature control switched on and stirrer running

To test the gassing, proceed as follows:

Procedure

1. If applicable, slowly open the rotameter needle valve.
2. If applicable, set a low setpoint in the appropriate parameter *Flow* (depending on the configuration) and switch the parameter on.
3. If applicable, ensure that all other gas parameters (e.g. *Gas-mix*, *GM Flow* etc.) are switched off.

If the gassing is working, air bubbles now form in the water in the culture vessel.

7.7.6 End of Test

After all parameter setpoints have been reached, the test can end here.

Proceed as follows:

Procedure

1. Stop the bioreactor on the operating panel and shut down the system.
2. Switch off the device at the power switch.



ATTENTION

Switching the device off at the power switch without previously stopping the bioreactor and shutting down the system on the operating panel may lead to damage of the operating panel!

3. Shut off the supply lines.
4. Empty the culture vessel.

Before Cultivation

8 Before Cultivation

The following chapters describe all the preparatory work before starting the cultivation process. This essentially comprises:

- Preparing and autoclaving the culture vessel:
 - Checking the gaskets (O-rings) on component parts and culture vessel
 - Mounting component parts
 - Filling or moistening the culture vessel
 - Preparing sensors and other accessories
 - Autoclaving
- Connecting the culture vessel and preparing for cultivation:
 - Connecting the cables and hoses between the culture vessel and the basic unit
 - Filling the vessel if necessary
 - Preparing sensors and other accessories



INFORMATION

The descriptions in the following chapters always refer to all available culture vessels. For practical reasons, however, the descriptions and instructions for the culture vessel usually refer to a single vessel.

8.1 Preparing and Autoclaving the Culture Vessel

All accessories required for later cultivation must be prepared and mounted accordingly and autoclaved together with the culture vessel.

8.1.1 Checking Gaskets (O-Rings)

O-rings are used to seal all openings on the vessel and top plate. The top plate, its ports and all accessories are thus equipped with O-rings. Before every use, the O-rings must be checked that they are present, undamaged and correctly seated. Damaged O-rings must be replaced.




INFORMATION

Wet the O-rings with 70% alcohol or a little water to facilitate removing and replacing O-rings or accessories with O-rings. Do not use silicone grease; this can affect sterilization results.


Before Cultivation

Carry out this check as follows:

Procedure

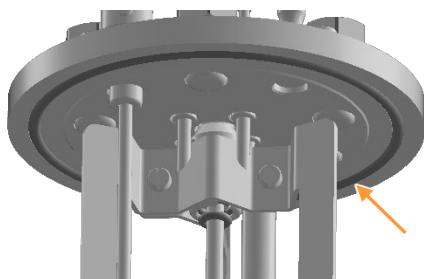

1. Check the O-ring for sealing the top plate for damage and for its correct position: it must be firmly seated in the groove on the inside of the top plate.
If necessary, insert it correctly.

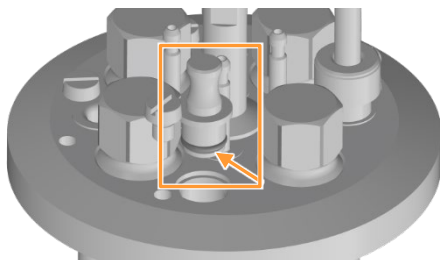

2. Ensure that every built-in part is equipped with an intact O-ring: Check that the O-rings are correctly positioned and are undamaged. If necessary, reposition or replace.

If built-in parts are fitted into other built-in parts (clamping adapter), there must also be an O-ring between them.




INFORMATION

Septum collars are sealed with a septum. No O-ring is used.

8.1.2 Mounting the Bearing Holder in the Top Plate


To mount the bearing holder in the top plate, proceed as follows:

Procedure

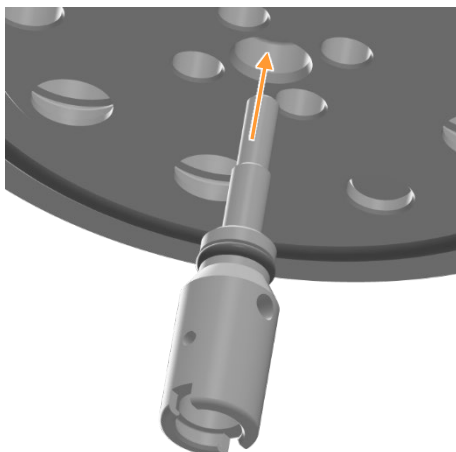

1. Insert the bearing holder equipped with the O-ring into the opening in the centre of the top plate.
The O-ring offers slight resistance during insertion.

Before Cultivation

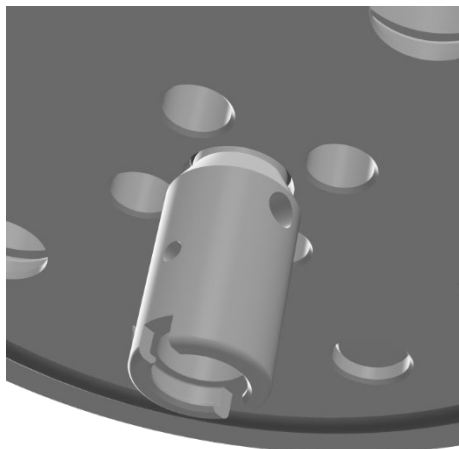


2. Make sure that the bearing holder is inserted into the top plate up to the stop.

8.1.3 Mounting the Addition Port Adapters and Hose Holder

To mount the four addition port adapters and fix them to the hose holder, proceed as follows:

Procedure

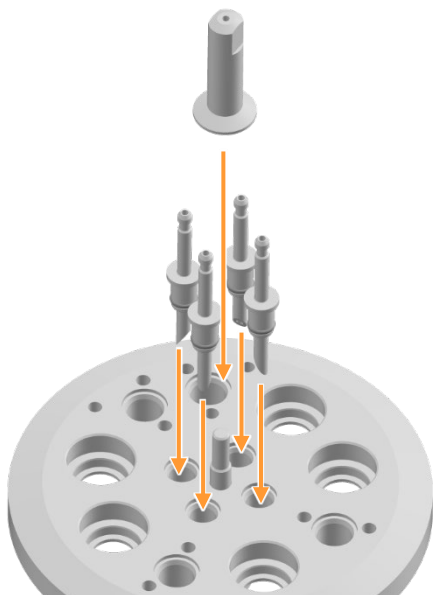


1. Insert the addition port adapters with the needle tips facing outward into the ports.
If one or more ports are not supposed to be used, use blanking plugs instead.
2. Screw the hose holders onto the thread of the bearing holder.
This affixes the stirrer shaft and addition port adapters or blanking plugs in the top plate.

The wire of the hose holder (not depicted) can be inserted now or when preparing the reagent bottles.

8.1.4 Mounting the Stirrer Shaft

To mount the stirrer shaft into the bearing holder, proceed as follows:

Procedure

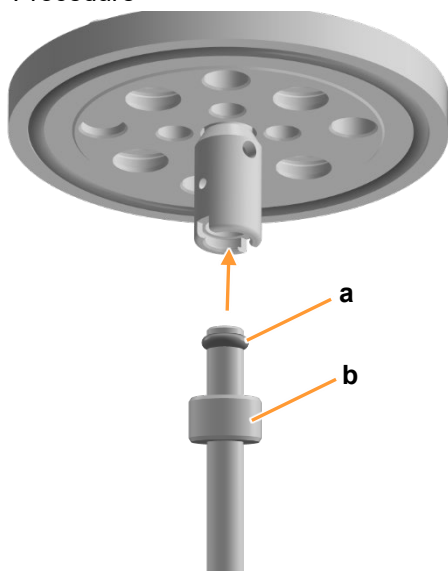


1. Insert the stirrer shaft equipped with O-ring (a) and stirrer shaft bearing (b) into the bearing holder.




INFORMATION

For 750 mL culture vessels, the bearing holder is welded to the baffles.

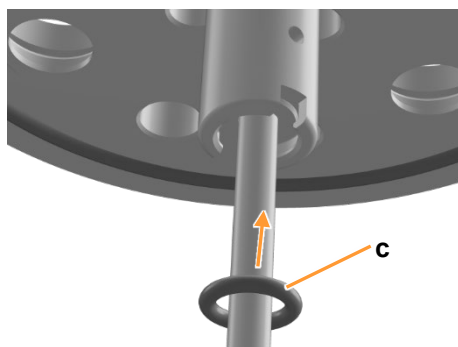


2. Slide the O-ring (c) onto the stirrer shaft.

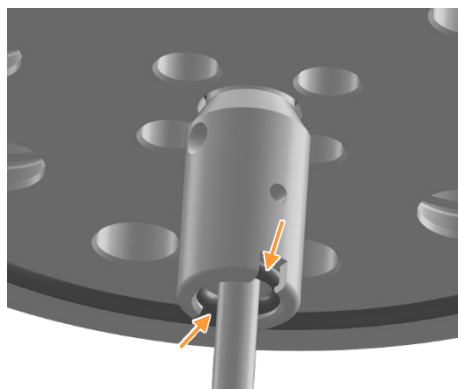

3. Carefully push the O-ring into the groove in the bearing holder with your finger; if necessary, use a small key/pen (not pointy or sharp-edged!).

This is used to hold the stirrer shaft bearing in place in the bearing holder.

Before Cultivation

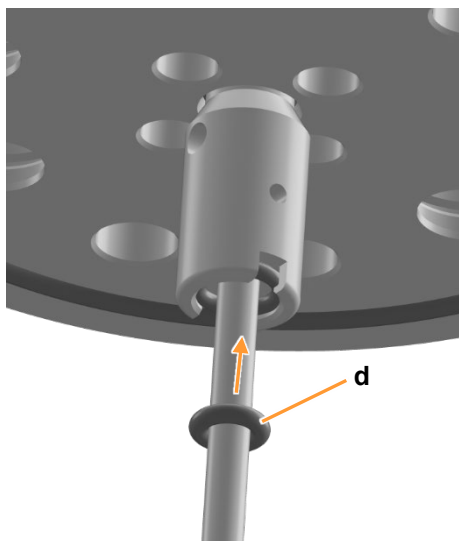

4. Slide the small O-ring (d) in front of the bearing holder.
This prevents the stirrer shaft from jumping out of the centering bearing at the lower end of the stirrer shaft.
The final position of the small O-ring is defined when setting the end clearance of the stirrer shaft, see chapter “Setting the End Clearance of the Stirrer Shaft”.


8.1.5 Mounting the Baffles

To mount the baffles, proceed as follows:

750 mL culture vessel: one-piece baffles

The baffles consist of one piece and are welded to the bearing holder.

Mounting takes place in the same way as for the bearing holder, see chapter “Mounting the Bearing Holder in the Top Plate”.


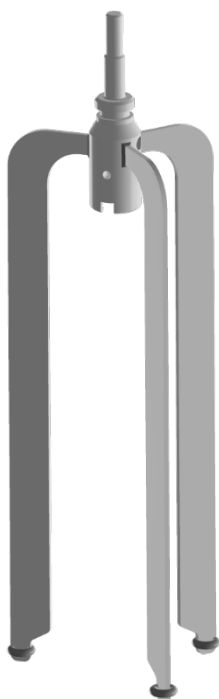


Before Cultivation

1400 mL culture vessel: two-piece baffles

Procedure

1. Loosen the slotted screws on the baffles.
2. Separate the two halves of the baffles.

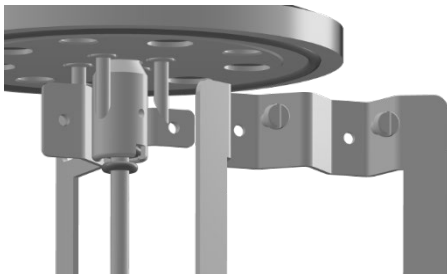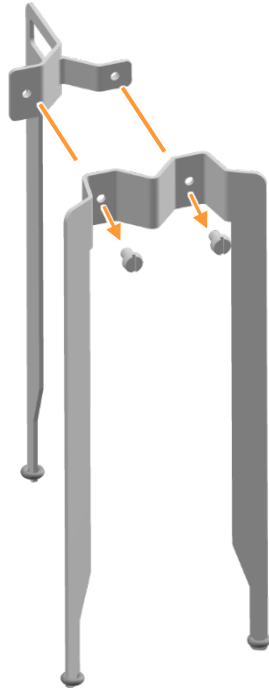

3. Place the halves of the baffles around the bearing holder. Ensure that the baffles are flush with the bottom of the bearing holder.
4. Affix them with slotted screws.

Before Cultivation

8.1.6 Mounting the Impeller, Flow Deflector and Magnetic Coupling

To mount the impellers, the flow deflector and the magnetic coupling, the individual parts must first be slid onto the stirrer shaft from below in the correct order before they can be affixed.

Special information on the magnetic coupling

Due to the very strong magnets in the magnetic coupling at the lower end of the stirrer shaft, ferromagnetic particles can be deposited on the stainless steel surfaces of the magnetic coupling. These particles are often not visible to the human eye. During autoclaving of the culture vessel, they decompose and cause visible stains, so-called flash rust.

As a general rule, mounting / disassembly of the stirrer shaft should always be carried out in an environment that is clean and, above all, free of any magnetic metals.




ATTENTION

Danger of material damage caused by magnetic fields. Magnetic fields can damage laptops, hard drives, ATM cards, data media and other items susceptible to magnetism.

Equipping the stirrer shaft

Slide the individual parts onto the stirrer shaft in the following order:

Procedure

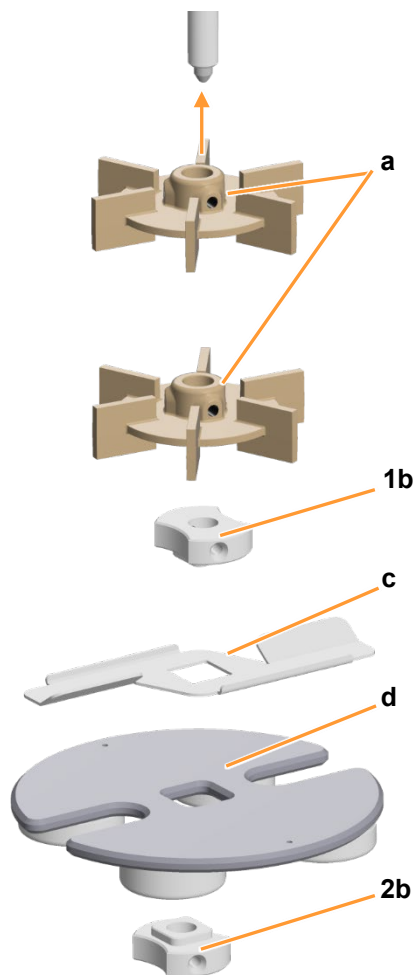




1. Both impellers (a).
2. First adjusting ring (1b).
3. Flow deflector (c).
4. Magnetic coupling (d).
5. Second adjusting ring (2b).

Before Cultivation

Attaching built-in-parts

To attach the individual parts to the stirrer shaft, proceed as follows:

Procedure

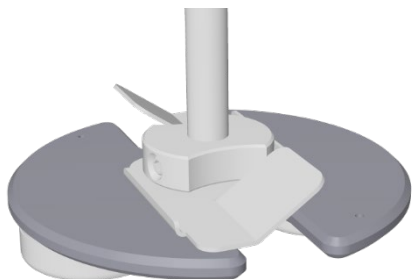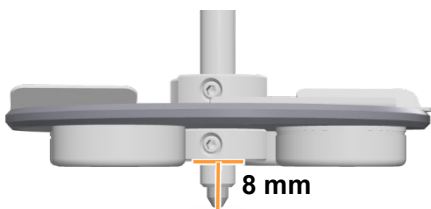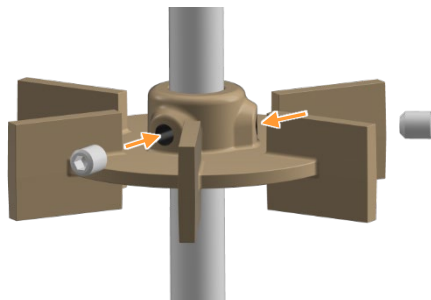

1. Set both impellers to the desired height.
2. Secure the impellers with the two grub screws.



INFORMATION

To avoid unnecessary foam formation, do not mount the impeller at the same height as the surface of the medium.


3. Place the lower adjusting ring so that its lower edge is at a distance of 8 mm to the tip of the stirrer shaft.
4. Secure the lower adjusting ring with grub screws.
5. Note the alignment of the flow deflector and magnet holder; adjust if necessary.
6. Secure the upper adjusting ring with grub screws.

8.1.7 Checking the Fit of the Centering Bearing of the Stirrer Shaft

To ensure that the stirrer shaft is kept stable, the centering bearing must be intact and anchored firmly.



- 400 mL and 1400 mL culture vessel: The centering bearing sits in the triangular plate on the base of the vessel.

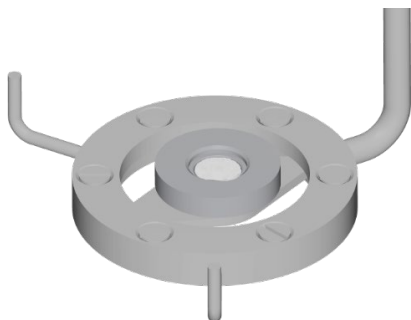Before Cultivation

- 750 mL culture vessel: The centering bearing sits in the aeration ring of the sparger.

8.1.8 Mounting Dip Tubes and Spargers


Straight spargers and dip tubes can be mounted to the outside of the vessel top plate. Curved spargers and dip tubes can only be mounted to the inside of the vessel top plate, this means that the vessel top plate is still removed.

Mounting to the inside of the vessel top plate is described here. During mounting, ensure that the sparger or the dip tube does not come into contact with other mounting parts.

**INFORMATION**

The correct mounting depth and alignment of the sparger result from the interaction of installation and adjustment of the longitudinal clearance of the stirrer shaft. Also observe the instructions in chapter "Positioning the Sparger in the Vessel" and "Adjusting the longitudinal Play of the Stirrer Shaft".

Proceed as follows:

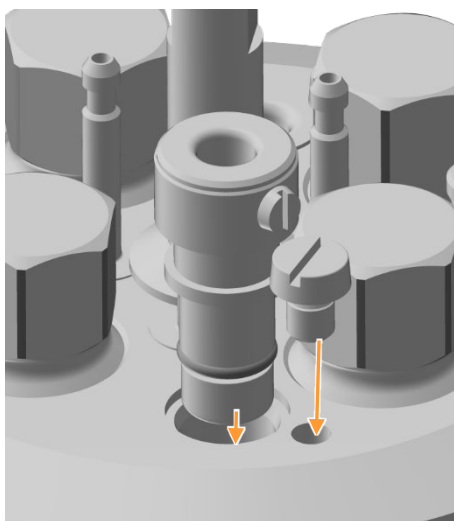
Procedure

1. Insert the clamping adapter equipped with an O-ring into the 10 mm port.
2. Gently screw in the slotted screw next to the port.

**INFORMATION**


Depending on the vessel size, two slotted screws exist for fastening.

Before Cultivation

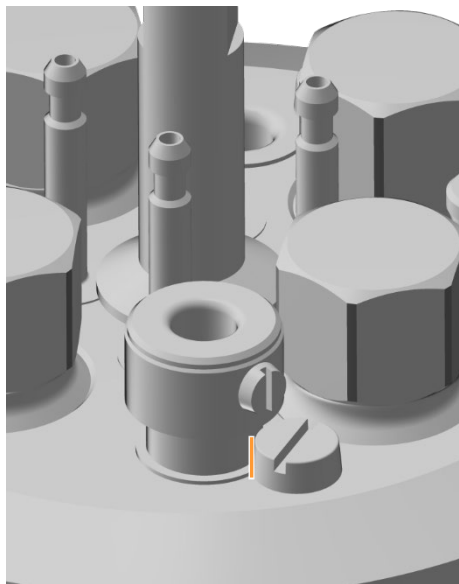

3. Insert the clamping adapter to the stop and fasten it in the port with (a) slotted screw(s).

The screw head or heads are located between the stop and the head of the clamping adapter.

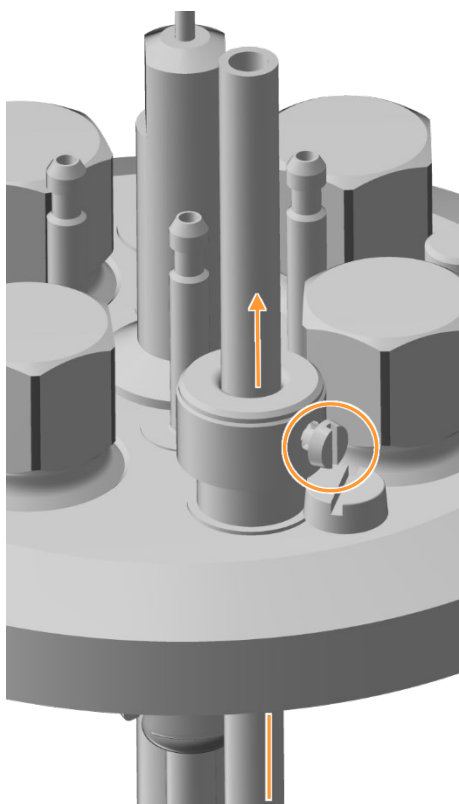

4. Slightly loosen the slotted screw on the clamping adapter.
5. Insert the sparger or dip tube into the clamping adapter from below.

6. Set the desired mounting depth, taking into account the alignment/position.
7. Tighten the slotted screw.

8.1.9 Positioning the Sparger in the Vessel


Since the sparger and location of the centering bearing are different for the three vessel sizes, the mounting and adjustment of the stirrer shaft and sparger are also slightly different.

Observe the following:

400 mL and 1400 mL culture vessels

It is recommended to first adjust the longitudinal play of the (correctly equipped) stirrer shaft so that it is correctly seated in centering bearing during operation.


The final mounting depth of the correspondingly aligned sparger can then be adjusted.

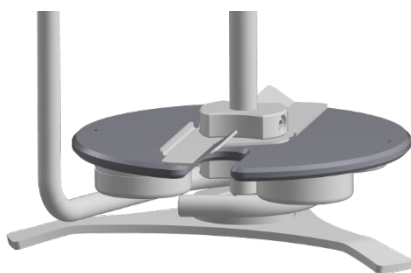


750 mL culture vessels

Since the centering bearing is located on the sparger's aeration ring, it is advantageous to first adjust the sparger's final mounting depth and its correct alignment in the vessel.

Then the longitudinal play of the (correctly equipped) stirrer shaft can be adjusted more easily.

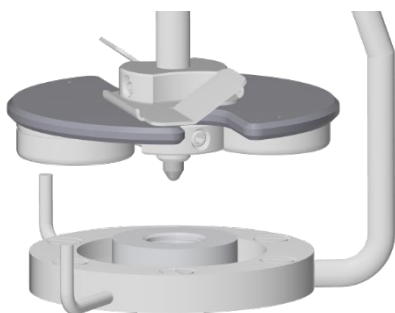

8.1.10 Adjusting the Longitudinal Play of the Stirrer Shaft

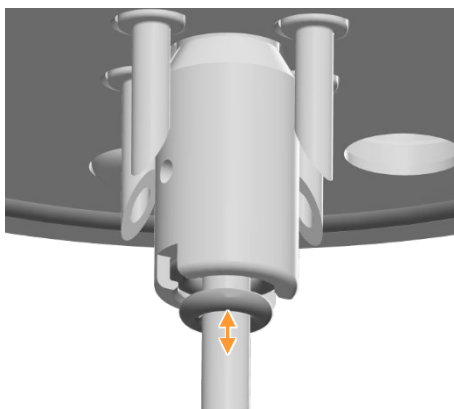

To prevent the stirrer shaft from jumping out of the centering bearing, the longitudinal play of the stirrer shaft must be adjusted correctly using the O-ring.



ATTENTION

Risk of damage to the centering bearing due to instable fit of the stirrer shaft!

If the stirrer shaft has too much vertical play, and is subsequently connected to the basic unit, the stirrer shaft can be pulled abruptly into the centering bearing by the magnets in the basic unit and thus damage the centering bearing.

Before Cultivation





INFORMATION

Before making the settings, read the notices in the “Positioning the Sparger in the Vessel” chapter.

Proceed as follows:

Procedure

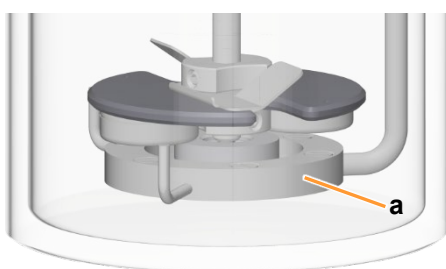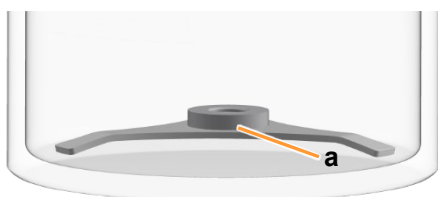

1. Ensure that the centering bearing is positioned in the glass vessel.
 - Culture vessel 400 mL and 1400 mL TV: The triangular plate (a) with the centering bearing sits on the bottom of the glass vessel, if necessary, insert it carefully.
 - Culture vessel 750 mL TV: The aeration ring (a) of the sparger is fitted correctly, aligned slightly above the base of the glass vessel, if not, adjust the sparger.
2. Carefully place the top plate onto the glass vessel from above and simultaneously insert the stirrer shaft tip into the centering bearing.

Putting on the top plate results in the correct mounting depth of stirrer shaft and sparger.
3. Carefully lift off the top plate and, if necessary, adjust the longitudinal play of the stirrer shaft by slightly shifting the small O-ring.

Before Cultivation**8.1.11 Moistening/Filling the Culture Vessel**

If in the culture vessel is to be autoclaved with the medium, the vessel can be filled before the top plate is put in position and the additional component parts are mounted.

Note the following about filling the culture vessel before autoclaving:

- Before autoclaving, only top up with heat-resistant media.
- During autoclaving, evaporation may result in a loss of volume and thus to increased salt concentration in the medium. If necessary, top up with sterile water.

**INFORMATION**

Development of steam is not possible when autoclaving an empty and dry culture vessel. Successful sterilization is not guaranteed.

Ensure that there is liquid in the culture vessel (approx. 10 mL of water per liter of total volume).

Before Cultivation


8.1.12 Putting on the Vessel Top Plate, Fastening with Clamping Ring


If built-in-parts such as stirrer shaft, sparger and, if applicable, dip tubes are mounted correctly and adjusted if necessary, the vessel top plate can be placed on the top and fastened with the clamp.

To do so, proceed as follows:



Procedure

1. Carefully place the vessel top plate on the glass vessel.

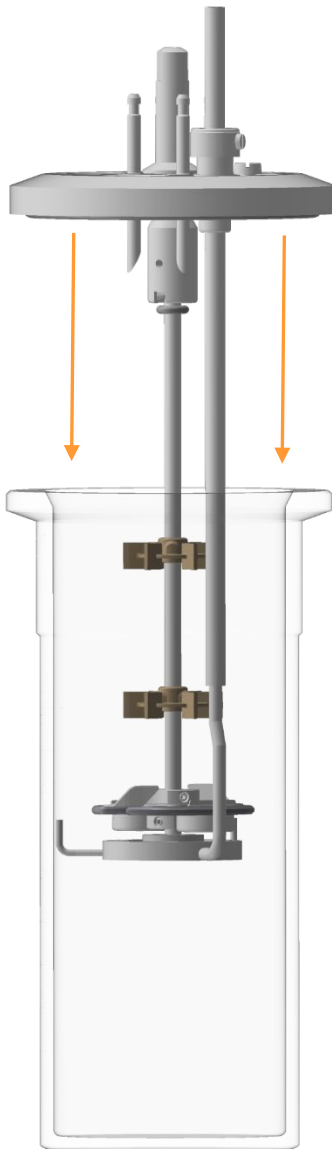


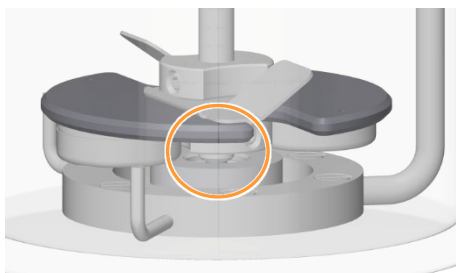Before Cultivation

In doing so, ensure that stirrer shaft sits in the centering bearing. For details on the interaction between stirrer shaft and sparger, see the chapters “Adjusting the Longitudinal Play of the Stirrer Shaft” and “Positioning the Sparger in the Vessel”.

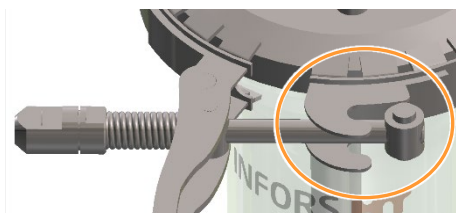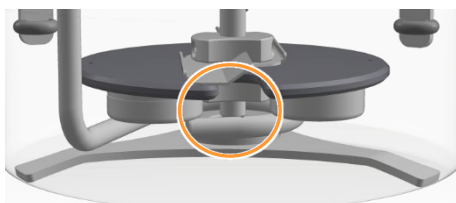

2. Place the clamping ring around the vessel top plate.
3. Use one hand to tighten the clamping ring around the vessel and use the other to hook in the threaded rod.

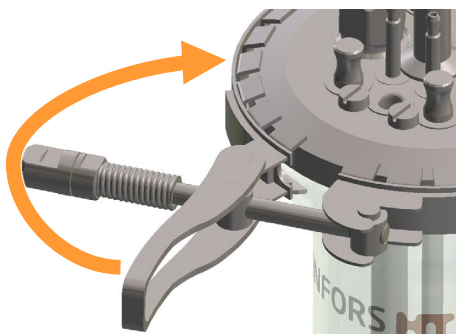

4. Hold the vessel on the clamping ring with one hand and close the fastener with the other hand.

**ATTENTION**


Ensure that the spring length is 21 mm (with the clamping ring closed) as set ex-factory to ensure sealing between top plate and vessel.

Before Cultivation

8.1.13 Inserting the Culture Vessels into the Vessel Holder

To be able to complete the remaining preparations, we recommend inserting the culture vessels into the vessel holder no later than at this point.


To this end, insert the culture vessel(s) into the centering ring(s) of the vessel holder from above.

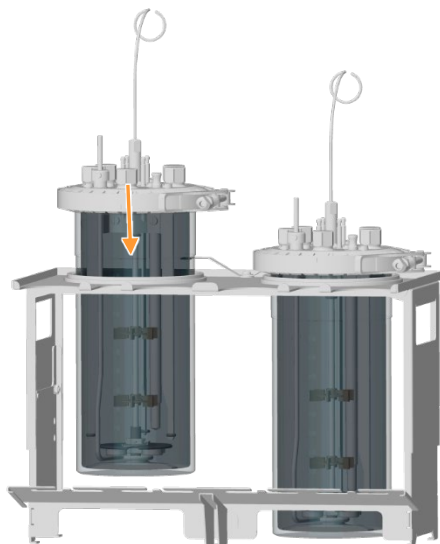

8.1.14 Mounting the Immersion Pocket for Temperature Sensor (Pt100)

Proceed as follows:

Procedure

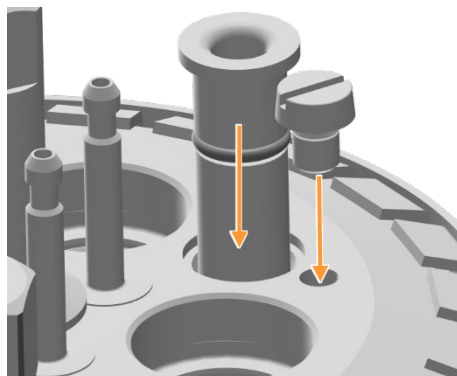

1. Insert the immersion pocket with the O-ring into the 10 mm port.
2. Fix it with the slotted screw(s).



INFORMATION


Depending on the vessel size, two slotted screws are available for fixation.

8.1.15 Mounting the Adapter Sleeve

Due to space constraints, culture vessels with a total volume of 400 mL must have an adapter sleeve mounted so that the exit gas cooler can be screwed into it.

To mount the adapter sleeve, proceed as follows:

Procedure

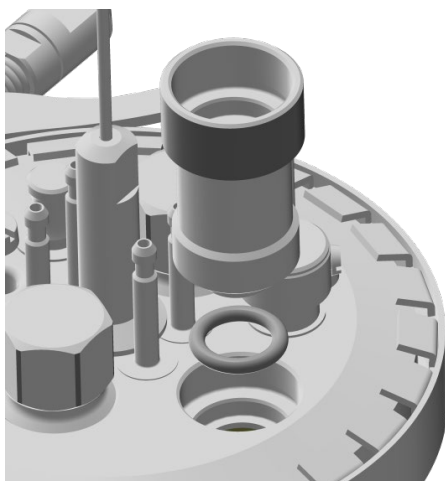


1. Equip the adapter sleeve with an O-ring.
2. Insert the adapter sleeve into the 12 mm/Pg13.5 port and screw it in by hand.

8.1.16 Mounting the Exit Gas Cooler


To mount the exit gas cooler, proceed as follows:

Procedure

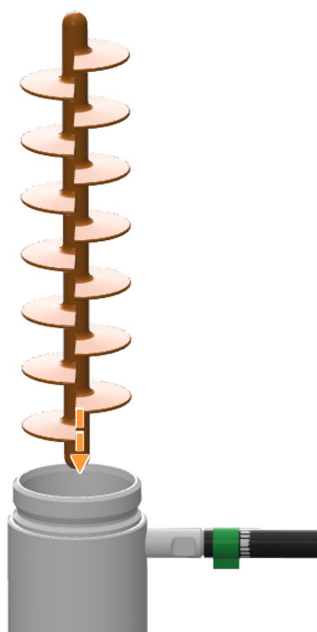


1. Insert silicone baffle into the exit gas cooler.

Before Cultivation

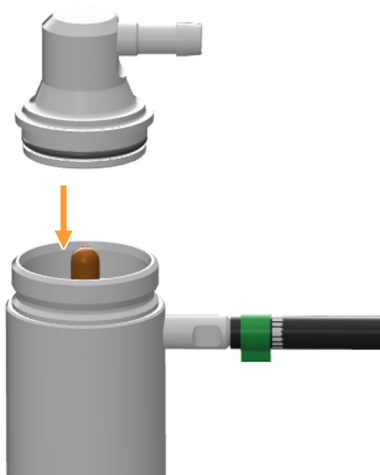


2. Place the lid with intact O-ring vertically onto the exit gas cooler by hand.
 - Align the exit gas pipe as far as possible on the same side as the hose connections.
 - The lid must sit straight and tight.

If necessary, wet the O-ring on the lid lightly with water to facilitate putting it on.

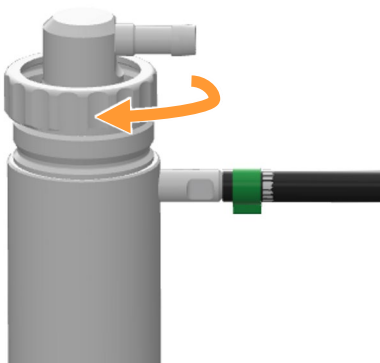

3. Attach the coupling nut and tighten it by hand in clockwise direction.

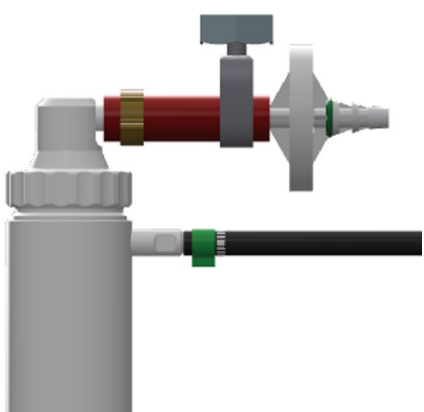

4. Equip the exit gas pipe with a piece of pressure hose (D = 6 x 11.9 mm) and a clean, dry exit gas filter. To do this, plug the inlet side (INLET) with the green marking in the piece of hose.
5. Secure the hose and exit gas filter with hose clamps (adjustable for exit gas filter).

6. Fit an O-ring to the thread of the exit gas cooler or fit it into the 12 mm / Pg13.5 port.
7. Screw the exit gas cooler into the port or, if applicable (400 mL culture vessels) into the adapter sleeve by hand.

Before Cultivation

8. Align the exit gas cooler to ensure that handling of other mounting parts is impaired as little as possible.
9. Check to ensure that the exit gas filter is fitted securely.
10. Cap the exit gas filter loosely with a little aluminium foil.

**INFORMATION**

A humidifier bottle with antifoam reagent can be installed between exit gas cooler and the exit gas filter if significant foam formation is expected.

Take the following into account for autoclaving:

- Only use a new, clean and dry exit gas filter and fix it in such a way that it cannot slip.
- ALWAYS keep the exit gas line - hose at the exit gas cooler with secured exit gas filter - open.

**CAUTION**

If pressure equalization does not take place via a top plate opening or the mounted exit gas cooler, overpressure or vacuum in the culture vessel may occur during autoclaving.


Before Cultivation

8.1.17 Mounting the Blanking Plugs

For mounting the different blanking plugs, proceed as follows:

Ø 10 mm ports

Procedure

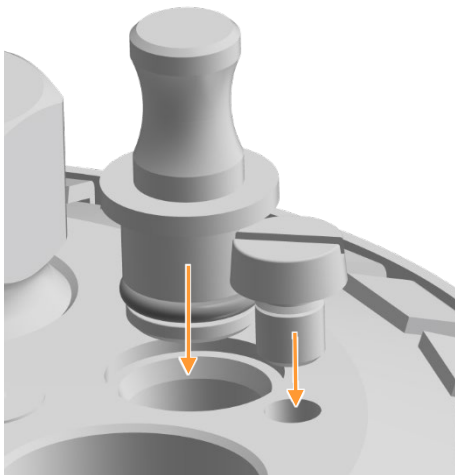

1. Insert the blanking plug with O-ring into the port.
2. Fix it with the slotted screw(s).




INFORMATION

Depending on the vessel size, two slotted screws are used.

Ø 12 mm ports

Procedure

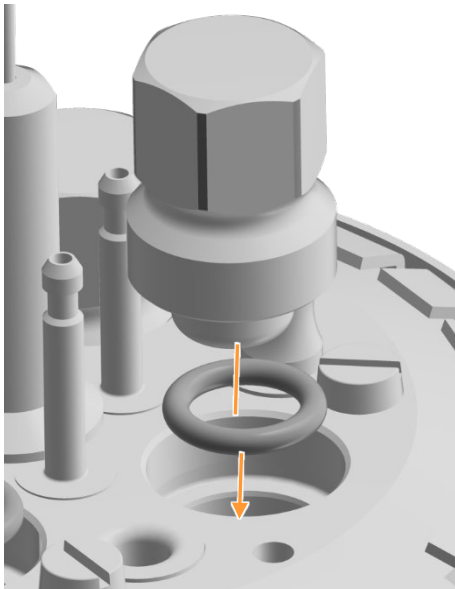

1. Insert an O-ring into the port.
2. Insert the blanking plug and screw it in by hand.
3. Tighten it with the hexagon socket spanner hand tight.

Before Cultivation**Ø 7.5 mm ports**

If a blanking plug is used instead of an addition port adapter, it must be fixed with the hose holder like the addition port adapter.

Procedure

1. Insert the blanking plug with O-ring into the port.
2. Screw the hose holder onto the thread of the stirrer shaft.
For more details refer to the chapter "Mounting Addition Port Adapter and Hose Holder".


8.1.18 Equipping the Port with a Septum Collar and Septum for Inoculation

For later inoculation with a syringe or inoculation needle, one of the 12 mm / Pg13.5 ports in the top plate must be appropriately prepared. It must be equipped with a septum collar and septum.

Proceed as follows:

Procedure

1. Ensure that there is no O-ring in the port; if there is, remove it.
2. Insert the septum (membrane) into the port.
3. Screw the septum collar into the port by hand.
4. Screw the blanking plug equipped with an O-Ring into the septum collar by hand.
If necessary, tighten it with the hexagon socket spanner hand-tight.

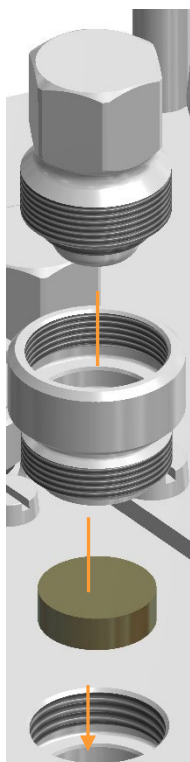

Before Cultivation

8.1.19 Preparing the Dip Tube/Addition Port Adapter for Inoculation

If later inoculation is to be carried out by means of a dip tube or addition port adapter, proceed as follows:

Procedure

1. Fit the dip tube with the clamping adapter or addition port adapter in the port.
2. Place a piece of silicon hose onto the dip tube/addition port adapter.
3. Equip the hose for a sterile hose connection. (Depending on the application: rapid coupling, sterile connector or weldable hose with sterile filter).
4. Secure the hose transition points with cable ties.



INFORMATION

An inoculation needle WITHOUT septum collar and WITHOUT septum can be used like an addition port adapter or a dip tube.

8.1.20 Preparing the Sensors

All sensors that come into contact with the medium are mounted before autoclaving and are sterilized together with the culture vessel.

Note the following about all sensors:

- Mount all sensors by hand – do not use any tools!
- Mount the sensors in such a way that they cannot come in contact with other built-in-parts or the glass vessel.
- If the mounting depth is adjustable (mounting with sensor holder/clamping adapter), make sure the mounting depth is set correctly prior to autoclaving, as later adjustment represents a contamination risk.

pH sensor

Calibrate the pH sensor before mounting and autoclaving.

pO₂ sensor

Mount the pO₂ sensor in such a way that it has good access to the flow and there is no risk of bubbles collecting.

Before Cultivation**Analog pH and pO₂ sensors**

Cover the sensor heads of the analog pH sensors and pO₂ sensors with aluminium foil during autoclaving.

Digital pH and pO₂ sensors**ATTENTION**

Risk of damage to the digital pH and pO₂ sensors. Covering the sensor heads with aluminium foil during autoclaving may lead to water gathering under the film, thus damage the contacts on the sensor head.

Sensor heads of the digital pH and pO₂ sensors should **NOT** be covered with aluminium foil during autoclaving.

For details on the safety, technical data, usage and maintenance requirements for the pH and pO₂ sensors, see the separate documentation provided by the manufacturers.

8.1.20.1 Calibrating the pH Sensor

The calibration of a pH sensor must always be carried out before autoclaving. This is done on the operating panel and is described in detail in the separate operating manual of the touch screen software.

Procedure**1. Connect the sensor cable.**

The different sensor and cable connections depending on the existing pH measurement system are briefly described in the chapter "Connecting the pH sensor".

2. Switch on the device at the power switch.

The operating panel is switched on automatically and the system is started.

3. Calibrate the pH sensor in accordance with the detailed description in the operating manual of the touch screen software.**INFORMATION**

If the pH sensor has already been calibrated externally, the bio-reactor will use this data and the calibration procedure in the touch screen software is not necessary. This only applies to the digital pH sensors.

Before Cultivation

8.1.20.2 Mounting a Sensor into a 12 mm Port

Depending on sensor length and vessel volume, sensors can be directly screwed into 12 mm / Pg13.5 ports. To do so, proceed as follows:


Procedure

1. Slide the O-ring onto the sensor.



INFORMATION

When mounting sensors in a 12 mm/Pg13.5 port, only use the O-ring of the vessel top plate port! Always remove any existing sensor O-rings and support rings.

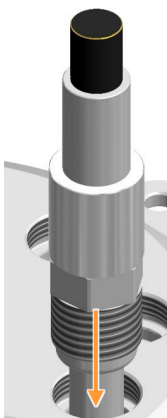

2. Insert the sensor into the port and tighten it by hand.

8.1.20.3 Mounting Sensors with Sensor Holder

To enable adjusting the mounting depth of a sensor in a 12 mm/Pg13.5 port, a sensor holder must be used for mounting.

Proceed as follows:


Procedure



1. On the sensor holder, lightly loosen the grub screw in the support guide with the key.

Before Cultivation

2. Pull the support guide from the guide bar.
3. Insert the sensor into the support guide and tighten it.

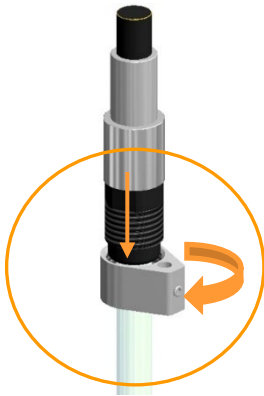

4. Insert the sensor into the hollow screw with the thread pointing in the downward direction.
5. Fit the fork of the guide bar into the groove of the hollow screw.
6. Push the hollow screw and the guide bar together upwards and insert the guide bar into the hole of the support guide.




Before Cultivation



INFORMATION

When mounting sensors in a 12 mm/Pg13.5 port, only use the O-ring of the vessel top plate port! Always remove any existing sensor O-rings and support rings.

7. Slide the O-ring onto the sensor and insert the sensor into the port.
8. Adjust the sensor to the desired mounting depth.
9. Screw the sensor on the hollow screw into the port and tighten it.
10. Tighten the grub screw in the support guide with the key.

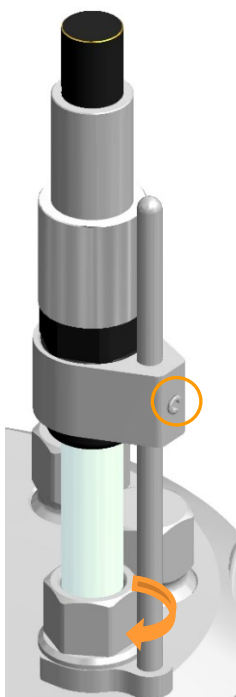

8.1.20.4 Mounting the Antifoam Sensor

Note the following points for mounting:

- The antifoam sensor is equipped with transparent insulation that must be intact, as otherwise a continuous signal “Foam/li-
quid detected” may be generated.



ATTENTION

If the sensor is fixed too tightly in the clamping adapter, or the mounting depth of the sensor is changed while the screw on the clamping adapter is tightened, the sensor insulation may be damaged.


Before Cultivation

- The sensor head must not touch the clamping adaptor, otherwise a continuous short-circuit is generated, indicating “Foam/liquid detected”.
- The clamping adaptor on the sensor must be equipped with an intact O-ring.

Procedure


Standard antifoam sensor, mounting in 10 mm port

1. Remove the protective cap from the sensor.
2. Ensure the clamping adaptor is equipped with an O-ring, fit one, if necessary.
3. Insert the sensor into the port.
4. Fix the clamping adaptor with the two slotted screw(s).

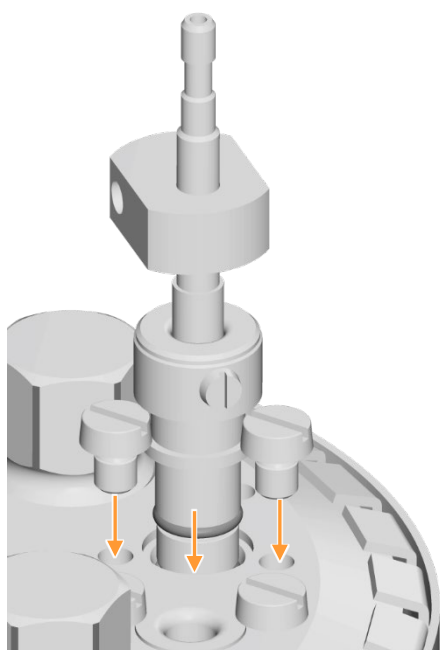

INFORMATION

Depending on the vessel size, one or two slotted screws are used.

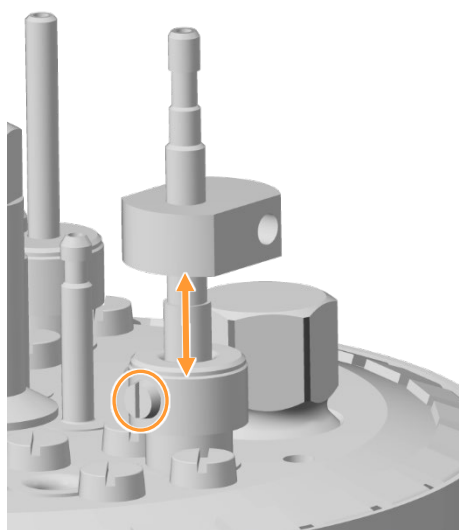

5. Loosen the slotted screw at the clamping adaptor.
6. Set the desired mounting depth of the sensor carefully.
7. Tighten the slotted screw carefully.


Before Cultivation

Optional antifoam sensor, mounting in 12 mm / Pg13.5 port

Proceed as follows:


Procedure

1. Remove the protective cap from the sensor.
2. Equip the clamping adapter with an O-ring or place it in the port.
3. Insert the sensor into the port.

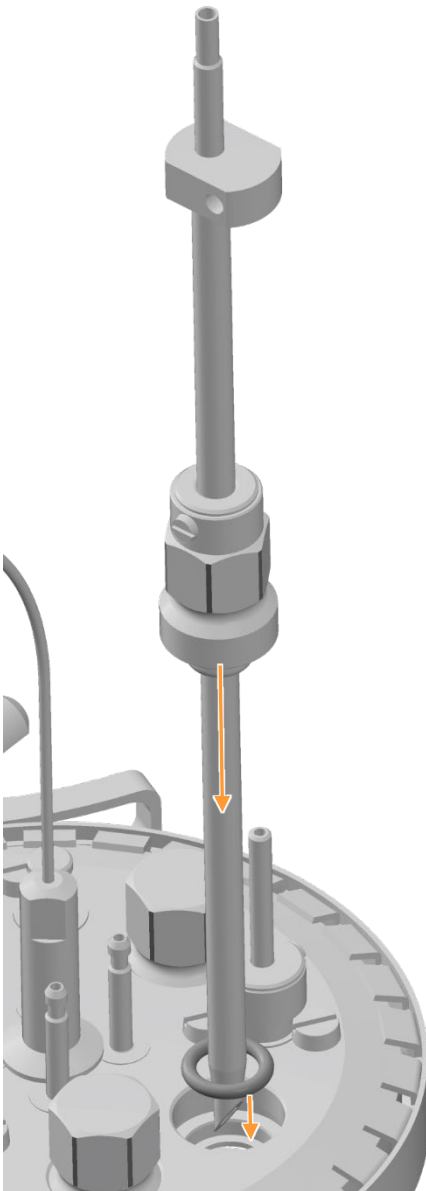

4. Tighten the clamping adapter by means of the hexagon socket spanner hand tight.

Before Cultivation

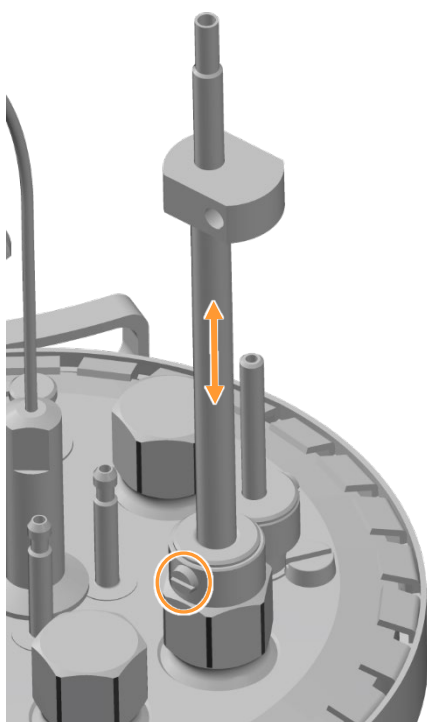

5. Loosen the slotted screw at the clamping adapter.
6. Set the desired mounting depth of the sensor carefully.
7. Tighten the slotted screw carefully.

8.1.21 Preparing the Super Safe Sampler



INFORMATION

The following figures are for general purposes of comprehension.

In order to prepare the Super Safe Sampler sampling system for autoclaving, proceed as follows:

Procedure



1. Attach the hose of the valve group on the dip tube.
2. Secure the hose with a cable tie.

Before Cultivation



3. Tighten the sample valve carefully by hand in a clockwise direction.

This ensures that the non-return valve/sample valve screw connection is tight.



4. Turn the sterile filter carefully by hand in a clockwise direction.

This ensures that the non-return valve/sterile filter screw connection is tight.



5. Cover the valve group loosely with aluminium foil.

6. Clamp off the hose on the dip tube.

8.1.22 Mounting the Sparger Hose and the Inlet Air Filter

The sparger must be equipped with the hose and inlet air filter before autoclaving.


To do so, proceed as follows:

Procedure

1. Cut a short piece of silicone hose.
2. Fit the inlet air filter, marked in red, to one hose end.
The nozzle with the red INLET marking remains exposed.



3. Connect the open end of the silicone hose to the sparger.

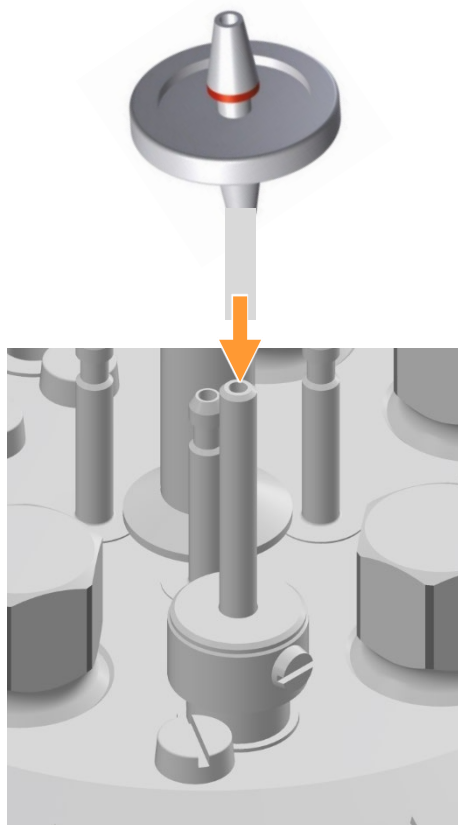

4. Secure the ends of the hose with the cable tie.

Before Cultivation

5. Clamp off the silicon hose with a hose clamp.
6. Lightly cap the inlet air filter with aluminium foil.

8.1.23 Preparing the Gassing Hose Line on the Basic Unit

An appropriate hose line must be prepared on the basic unit in order to connect the sparger to the gassing after autoclaving.

Proceed as follows:

Procedure

1. Cut a piece of thick walled silicone hose (Ø 4 x 7 mm, in the starter kit).
Choose its length so that the hose connection between sparger and gas supply on the basic unit does not have any tension or kinks.
2. Fit the hose to the hose nozzle of the gassing unit ¹⁾ on the basic unit.
3. Secure the hose with cable ties.



INFORMATION

If using a gas mixture and depending on the configuration and gassing strategy, further hoses must be connected to additional gassing units ¹⁾ and merged using one or several Y-pieces.

¹⁾ *depending on the chosen gassing strategy, this can be rotameter(s), mass flow controller(s), solenoid valve(s).*

8.1.24 Calibrating the Pumps

Not calibrated pumps show the duration in seconds and the number of rotations. If the delivered volume (in mL) shall be indicated instead, the pumps must be calibrated before autoclaving.

A detailed description of how to calibrate the pumps can be found in the separate operating manual of the touch screen software.

8.1.25 Preparing the Reagent Bottles, Pumps and Hoses



ATTENTION

Damaged hoses and/or clogged filters may lead to undesired pressure conditions in the reagent bottles.

- Ensure each reagent bottle is equipped with an open pressure equalization line with a clean and dry filter.
- Only use clean, intact hoses and ensure they are firmly attached.

The following sections contain a detailed description of how reagent bottles are equipped properly and connected to the pumps and culture vessel. Note that one reagent bottle is intended for two culture vessels.

Proceed as follows:

Procedure

1. Cut two long silicone hoses, $\varnothing = 2 \times 6$ mm (for details see main chapter “Accessories”, chapter “Reagent Bottles”) per pump.



INFORMATION

The length of the silicone hoses must be selected to ensure that the hose connections between the reagent bottles, pumps and culture vessel do not have any tensions or kinks.

2. Thoroughly rinse the silicone hoses with distilled water.

3. Connect the silicone hoses and pump hoses of the pump heads with hose connectors.



INFORMATION

Note that the direction of rotation of the pumps is counter-clockwise in operational state.

4. Secure with cable ties.




Before Cultivation

Connection between pumps and culture vessel

Proceed as follows:

Arbeitsschritte

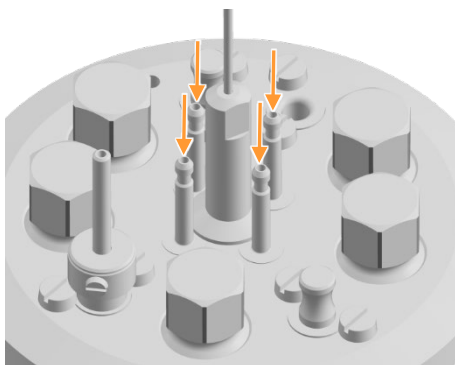

1. Fit silicone hoses for base, acid and feed to the addition port adapters and secure them with cable ties.

2. Attach the silicone hoses of the antifoam pump to the mounted antifoam sensor in the culture vessel and secure it with a cable tie.

Connection between reagent bottles and pumps

Proceed as follows:

Procedure

1. Ensure that a hose is fitted inside the reagent bottles at the exposed hose connections (without filter); fit one if not:
 - a) the hose ends do not touch the bottom of the bottle, otherwise the hoses may get sucked against the bottom and will no longer be able to pump liquid.
 - b) the hose ends are cut diagonally. In this case the hose ends can touch the bottom of the bottle.
2. Label the reagent bottles in accordance with their content.
3. Depending on the application: Fill the reagent bottles with reagents and reclose them with their lid.



ATTENTION

Usage of the highly corrosive hydrochloric acid HCl as reagent leads to damage to components made of stainless steel such as e.g. component parts or the top plate.

Use only non-corrosive acids, e.g. phosphoric acid, instead.

Before Cultivation**INFORMATION**

Fill reagent bottles with heat-resistant reagents only. Sterilize non-heat-resistant feed solution separately and only transfer it to the reagent bottle after sterilizing.



4. Place the reagent bottles in reagent bottle and pump holders.
5. Attach the correct silicone hoses to available hose connections of each reagent bottle.
6. Secure the hoses with cable ties.
7. Close silicone hoses with clamps as close as possible to the hose connections of the reagent bottles to ensure that no reagent can flow into the culture vessel.
8. Ensure that:
 - each reagent bottle is connected with the appropriate pump according to its contents. (Base to base pump, etc.).
 - filters are clean and dry; short hose line is open.
9. Cap the filters loosely with aluminium foil.

8.1.26 Sterile Hose Connections

If additional vessels are needed and these can only be connected to the culture vessel after autoclaving, such as vessels for the inoculum or bottles for sampling etc., rapid couplings (male/female), sterile connectors or – if weldable hoses are used – a hose welding device can be used to form a sterile connection.


Before Cultivation

The connection pieces must be fitted to the appropriate hoses before autoclaving. Rapid couplings are connected after autoclaving in a sterile workbench. Sterile connectors and hose welding devices allow sterile connecting without a sterile workbench.

8.1.27 Removing the Pump Heads

To remove the pump heads from the basic unit, proceed as follows:

Procedure

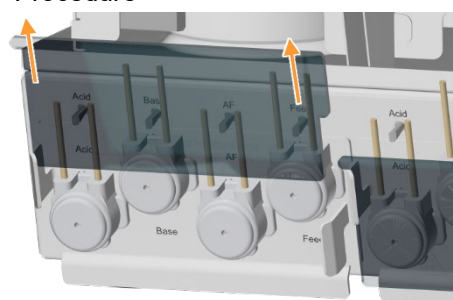

1. Pull up the pump cover plate and remove it from the holder.




INFORMATION

The pump cover plate serves only as a protective device in operating mode. It is not heat proof and therefore it may not be autoclaved.



2. Pull the mounting plate with the pump heads off the drive shafts by the two handles.

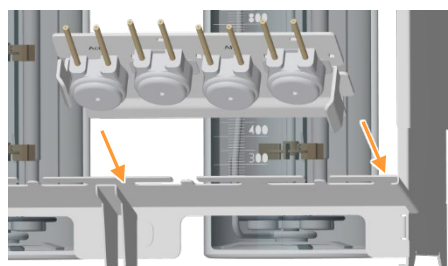

3. Fit the mounting plate with the pump heads onto the vessel holder.

4. Lift the vessel holder by means of its handles and transport the culture vessels together with the reagent bottles and pump heads as a unit to the autoclave

Before Cultivation**8.1.28 Checklist Before Autoclaving**

Check and ensure the following items before autoclaving:

Culture vessel

All necessary O-rings are fitted.

All unused ports are closed with blanking plugs

Port for inoculation (with syringe) is equipped with septum, septum collar and blanking plug

There is liquid in the culture vessel (autoclavable medium or approx. 10 mL water per liter working volume).

Reagent bottles, hoses and pumps

Reagent bottles are exclusively filled with autoclavable liquids, correctly labelled and connected with the culture vessel and the pump heads via hoses.

Reagent bottles are equipped with filters for pressure equalization

Reagent bottles are placed in support on vessel holder and pump heads with mounting plate are attached.

Super Safe Sampler

The valve group is connected to the dip tube in the culture vessel by means of a hose.

The valve group is lightly capped with aluminium foil.

Sparger and exit gas cooler

The sparger is equipped with a hose and an inlet air filter.

The exit gas cooler is equipped with a new securely fastened exit gas filter.

Filters and hoses

All filters are clean, dry and lightly capped with aluminium foil.

There are no open hose ends.

All hose transition points are secured with an autoclavable cable tie or hose clamp to prevent them from slipping.

Hoses on the reagent bottles, for sampling and the gassing system (sparger) are clamped off with hose clamps.

The exit gas hose is **NOT** clamped off.

The hoses are undamaged; the hose lines show no kinks and are not able to kink.

Before Cultivation

Sensors

All sensors required are mounted and, if necessary, calibrated.

The antifoam sensor is mounted, set for the correct mounting depth and connected to the correct reagent bottle.

The temperature sensor of the autoclave is inserted into the immersion pocket for the temperature sensor of the culture vessel.

pH and pO₂ sensors:

- ANALOG: are covered with aluminium foil.
- DIGITAL: are **NOT** covered with aluminium foil.

8.1.29 Autoclaving

Before cultivation starts, the culture vessel is autoclaved in accordance with the application in question. The culture vessel can be autoclaved with or without medium.

Adhere to the following:

- Never autoclave the culture vessel dry; see also the chapter “Moistening/Filling the Culture Vessel”.



INFORMATION

Development of steam is not possible when autoclaving an empty and dry culture vessel. Successful sterilization is not guaranteed.

Ensure that there is liquid in the culture vessel (approx. 10 mL of water per liter of total volume).

- If necessary, pump off any remaining water after autoclaving by means of the dip tube.
- Sterilize all liquid, heat-instable components separately and add them after autoclaving.
- If the medium is autoclaved in the culture vessel, you may then need to add sterile water to make up the volume.

Proceed as follows to autoclave the culture vessel:

Procedure

1. Place the culture vessel including accessories in its holder into the autoclave.
2. Ensure that the culture vessel and the accessories do not touch the inner wall of the autoclave.

Before Cultivation

3. Ensure that the exit gas filter is open.
4. Insert the temperature sensor of the autoclave into the immersion pocket for the temperature sensor.
5. Select the program for liquids.
6. Autoclave the culture vessel in accordance with the operating manual of the autoclave manufacturer.


8.2 Connecting the Culture Vessel and Preparing the Cultivation

As soon as the culture vessel(s) with accessories have cooled down sufficiently, they can now be inserted into the vessel holder on the basic unit and the various cable and hose connections between the basic unit and the culture vessel can be established.


8.2.1 Fixing the Culture Vessels to the Basic Unit

To insert and fix the culture vessels to the basic unit, proceed as follows:


Arbeitsschritte

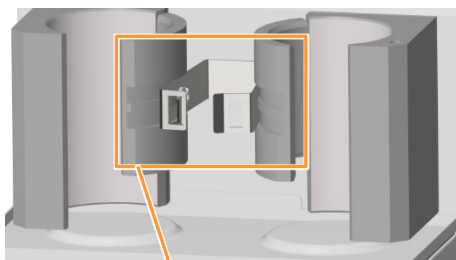

1. Press the brackets between the thermal blocks together on the basic unit until they snap into place.

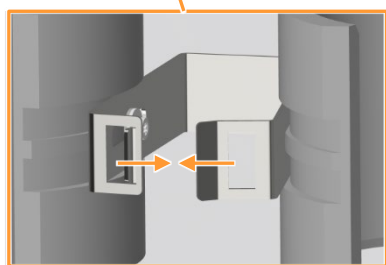

Before Cultivation

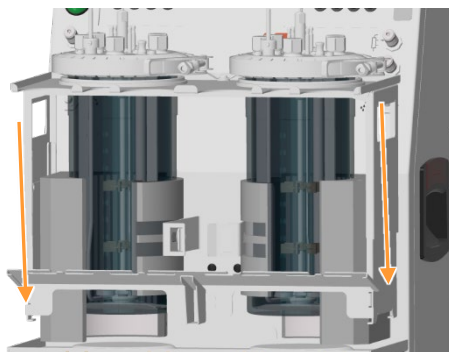

2. Insert the vessel holder with culture vessels into the thermal blocks from above.

3. Hold both brackets between the thermal blocks and simultaneously press the left bracket inwards.



INFORMATION

Do not pull the right bracket forward!


The culture vessels are fixed in the thermal blocks now.

8.2.2 Mounting the Pump Heads

To mount the pump heads on the basic unit, proceed as follows:

Procedure

1. Pull the mounting plate with the pump heads out of the holder on the vessel holder.

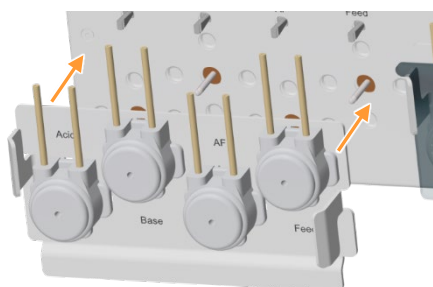

2. Push the mounting plate with the pump heads onto the pump motor drive shafts.

3. Plug the pump cover plates into the holders and fit the hoses into the hose holders.

8.2.3 Filling the Reagent Hoses

In order to prepare the reagent hoses for operation, they must be filled with reagent. This can either be done using the rocker switches of the pumps on the basic unit or via the touch screen software.



INFORMATION

When using several devices at the same time, it is useful and time-saving to fill all reagent hoses simultaneously and automatically.

For details about filling via touch screen software refer to the separate operating manual of the touch screen software.



WARNING

When using heavily corrosive reagents (acids and bases), it is particularly important only to use suitable and undamaged hoses. They must also be securely fastened. Furthermore, the exit gas filter must not be blocked. This ensures that no pressure builds up and no reagent escapes due to burst hoses.

Observe the following points:

- Remove the clamps from the reagent hoses, before filling.
- Ensure that no reagent escapes into the culture vessel, if possible.


Filling via rocker switches

Proceed as follows:

Procedure

1. Switch the device on at the power switch.
2. Open the clamps on the reagent hoses.
3. Operate the rocker switches and manually fill the reagent hoses one after the other:

Before Cultivation

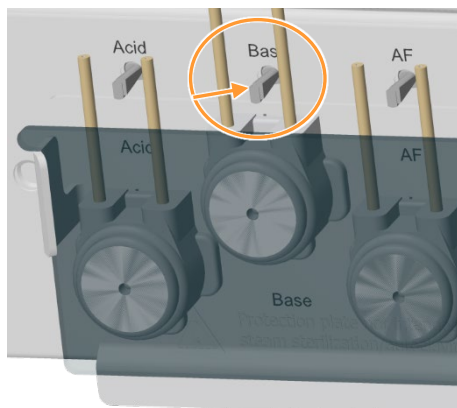

- Press the rocker switch to the right side: the pump runs forward (counter-clockwise), reagent is sucked in from the reagent bottle and is pumped in the direction of the vessel.
- Press the rocker switch to the left side: the pump runs backwards (clockwise), reagent is liquid is sucked in from the culture vessel and is pumped in the direction of the reagent bottle.

Release the rocker switch just before liquid visibly enters the addition port adapter(s), respectively the dosing needle of the antifoam sensor so that no reagent can enter the culture vessel.

8.2.4 Connecting the Gassing

To connect the sparger to the gassing, proceed as follows:

Procedure


1. Remove the aluminium foil from the inlet air filter.
2. Attach the gassing hose of the basic unit to the inlet air filter of the sparger and secure it with a cable tie.
3. Remove the clamp.

Before Cultivation**8.2.5 Connecting the Exit Gas Cooler**

To connect the exit gas cooler to the basic unit, proceed as follows:

Procedure

1. Remove the aluminium foil from the exit gas filter.
2. Insert the nozzles on the pressure hoses of the exit gas cooler into the rapid couplings on the basic unit in accordance with the symbols.

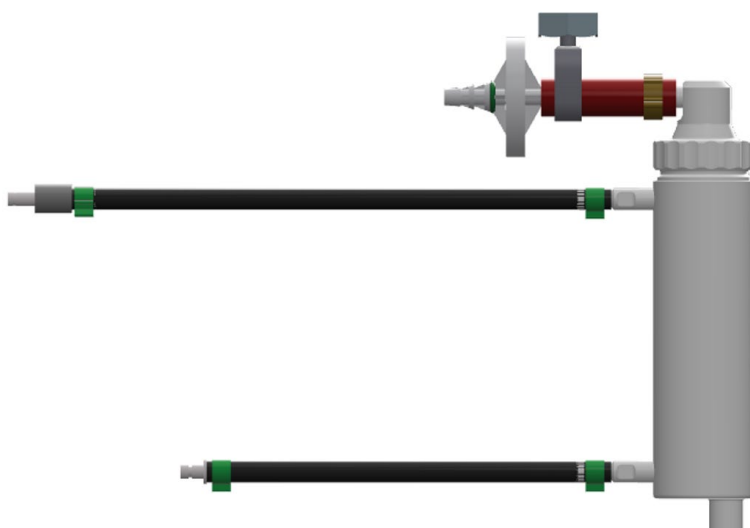**INFORMATION**

To facilitate connecting and disconnecting the exit gas cooler from the basic unit, put a little bit of silicone oil on the rapid couplings on the basic unit.

3. If necessary, change the default setting for water flow on the manual valve.

The exit gas cooler only works when the temperature control system is switched on (parameter *Temperature ON* in the touch screen software).

**INFORMATION**

If no exit gas cooler is used, close the valve for water flow of the exit gas cooler on the basic unit to avoid water leaking or seal the hose connections with the plugs provided.

Before Cultivation

8.2.6 Filling the Culture Vessel

Depending on the application, the vessel can be filled after autoclaving. To prevent foam formation during filling, add the medium via a dip tube.

To do so, proceed as follows:

Procedure

1. Sterilize the medium separately.
2. If necessary, pump off any water that remains in the culture vessel.
3. Establish a sterile hose connection between the culture vessel and the medium container.
4. Pump the desired quantity of medium into the culture vessel.
5. Clamp off the medium hose; if necessary, apply a welded seal.
6. Disconnect the medium container from the culture vessel; if necessary, retain it as a harvest or waste container.



INFORMATION

If the stirrer is turning on the surface of the medium, foam will be formed. For this reason, only switch on the stirrer if it is fully covered by medium.

8.2.7 Connecting the Temperature Sensor (Pt100)

The temperature sensor is not in direct contact with the medium.

Procedure

1. Insert the sensor into the immersion pocket in the vessel top plate as far as it will go.



CAUTION

Risk of burns and loss of property due to increased temperature!

The thermal block will overheat without an inserted temperature sensor and without liquid in the vessel. This can lead to burns and loss of property.

Before Cultivation

8.2.8 Connecting the Antifoam Sensor

Procedure




To connect the antifoam sensor, the two banana connectors of the sensor cable must be inserted as follows:

1. Insert the red banana plug into the connector on the sensor head.
2. Insert the black banana plug into the ground connection in the vessel top plate.

8.2.9 Connecting the pH Sensor

The sensor and cable connections of the pH sensors differ depending on the existing pH measurement system:

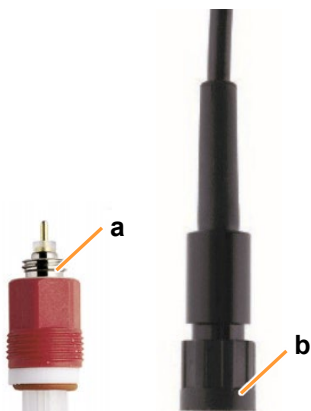


METTLER analog Type 405-DPAS-SC- K8S/120	Sensor head connection (a)	K8S
	Cable bushing (b)	AK9



ATTENTION

The sensor cable shield can be damaged by buckling or twisting. This may lead to faulty measurements.

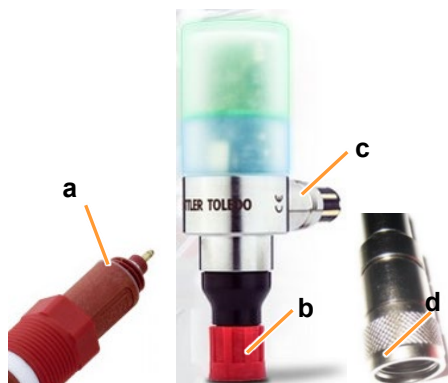

METTLER digital Type InPro 3253i	Sensor head connection (a)	ISM
	Cable bushing (d)	VP8
Head transmitter M100	Plug connection for sensor (b)	
	Plug connection for cable (c)	


Before Cultivation



HAMILTON digital Type Easyferm Plus ARC	Sensor head connection (a)	VP8
	Cable bushing (b)	VP8

8.2.10 Connecting the pO₂ Sensor

The sensor and cable connections of the pO₂ sensors differ depending on the pO₂ measurement system used:

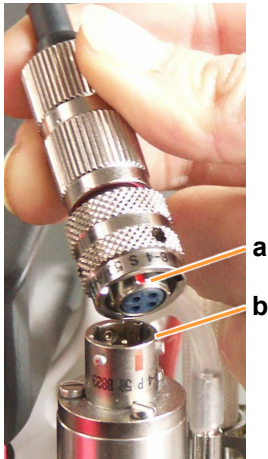


METTLER analog Type InPro 6820/25/080 (amperometric, polarographic)	Sensor head connection (a)	T-82
	Cable bushing (b)	T-82

**ATTENTION**

The sensor cable shield can be damaged by buckling or twisting. This may lead to faulty measurements.



METTLER digital Type InPro6860i	Sensor head connection (a)	VP8
	Cable bushing (b)	VP8

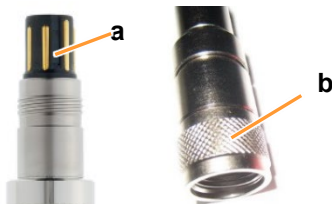

HAMILTON digital VisiForm RS485-ECS	Sensor head connection (a)	VP8
	Cable bushing (b)	VP8

8.2.11 pO₂ Sensor (Analog, Polarographic) Polarisation

Polarographic pO₂ sensors must be polarised at initial operation or after disconnection from the voltage source. Correct calibration is not possible otherwise.

For polarisation, the sensor cable must simply be connected to the pO₂ sensor and the device must be switched on at the main switch.

Duration of polarisation (= polarisation time) depends on how long the pO₂ sensor has been disconnected from the voltage source (= depolarisation time)

As a general rule: if depolarisation time > 30 minutes, the minimum polarisation time is 360 minutes.

More details about polarisation can be found in the separate documentation from the sensor manufacturer.

8.2.12 Calibrating the pO₂ Sensor

A 1-point calibration to 100 % is usually sufficient for exact measurement and should be carried out before each cultivation. If required, a 2-point calibration to 100 % and 0 is also possible.

A detailed description on the calibration can be found in the separate operating manual of the touch screen software.

8.2.13 Checking the Hoses and Hose Connections

Check and ensure the following items before each cultivation:

- Hoses show no kinks and are not able to kink.
- Hoses are undamaged and show no weaknesses.
- Gas hoses and connections do not show any leaks.
- Hose lines are as short as possible.
- Hoses are secured with cable ties and/or hose clamps.
- Only the pressure hoses supplied by the device manufacturer are connected as supply lines (water, gas) between the in-house connections and the device.

Cultivation

9 Cultivation

The following sections describe the work necessary for the performance of and after the completion of a cultivation, before the culture vessel with accessories is thoroughly cleaned and then prepared for another cultivation.

This essentially comprises:

- Preparing the medium, starting the bioreactor
- Sampling
- Inoculation
- Harvest
- Stopping the bioreactor, if necessary emptying the vessel
- Autoclaving the culture vessel and accessories

The requirement for the first item is that the culture vessel and accessories are autoclaved, cooled and connected to the basic unit. All cable and hose connections between the device and the culture vessel, including the reagent bottles, are present, pump heads are mounted and the reagent hoses are filled. Depending on the user specifications, the pO₂ sensor is already calibrated.



INFORMATION

The descriptions in the following chapters always refer to all available culture vessels. For practical reasons, however, the descriptions and instructions for the culture vessel usually refer to a single vessel.

9.1 Preparing the Medium

Before the first sampling, which usually takes place as a 'zero sample' before inoculation, and before the inoculation itself, the medium must be warmed to the desired temperature. If necessary, the pO₂ concentration and the pH are set. The time required for this depends on the working volume.

Set and activate the desired setpoint of the parameters in question on the operating panel, and start the bioreactor.

Depending on the specifications defined by the user, the pO₂ sensor is calibrated either before the vessel is filled with medium or afterwards, in the prepared medium.

**CAUTION**

If pressure equalization does not take place via a top plate opening or the mounted exit gas cooler, overpressure in the culture vessel may occur during cultivation as a result of warming, gassing or fermentation processes.

- Exit gas line - hose at the exit gas cooler with secured exit gas filter - **ALWAYS** keep open.
- Only use clean and dry exit gas filters.

For details about calibration and operation in general refer to the separate operating manual of the touch screen software.

9.2 Sampling

Samples are taken from the culture vessel to gain material for off-line analysis. The method of sampling can vary due to the different analyzes carried out by the operator.

The sampling procedure using the standard sampling system, Super Safe Sampler, is described below.

Before starting, observe the following:

**WARNING**

Culture solution could emerge from the vessel if the sample valve mechanically fails. This could lead to serious health risks in the event of applications with pathogenic organisms.

- When working with pathogenic organisms, always additionally clamp off the sampling hose with a metal (!) clamp.
- Only remove the clamp when sampling.
- Reattach the clamp before removing the syringe from the sample valve.

**WARNING**

Loose screws at components could lead to the penetration of unsterile air or contamination of the environment.

Before and after autoclaving: Check that all screws are tightly screwed in and, if necessary, tighten them manually.

Cultivation

If the sample is to be further aseptically processed, use a sterile syringe and sterile closing caps.

For details, see the main chapter “Accessories” chapter “Sampling System Super Safe Sampler”, section “Aseptic Sampling”.

Proceed as follows:

Procedure

1. Check that all screw connections of the valve group are tightly screwed in. If necessary, gently tighten the screw connections with two fingers.
2. Remove the clamp from the sampling hose.
3. If present: Remove the closing caps.
4. If desired: Disinfect the sample valve.
5. Screw open the Luer-Lock syringe on the sample valve.



6. Pull back the syringe plunger to remove the desired sampling volume.



If the dip tube was rinsed with air, air is sucked in first. Remove it as follows:

- a) Unscrew the syringe from the valve.
- b) Hold the syringe with the plunger downwards so that the medium remains in the syringe.
- c) Push the air out of the syringe.
- d. Screw the syringe onto the sample valve.
- e) Draw in again.

7. Attach the clamp to the sampling hose.

Rinsing the dip tube with sterile air

The dip tube and its sampling hose can be filled with sterile air after taking a sample.



INFORMATION

Only use a clean and dry syringe to avoid blocking the sterile filter. This syringe can be reused as often as desired, since air is provided via a sterile filter.

Procedure:



To do so, proceed as follows:

1. Insert the syringe onto the hose at the sterile filter and push air through.

The remaining liquid in the hose and in the dip tube is pushed back into the vessel.

2. Remove the syringe from the sterile filter to fill it with air again.
3. Repeat steps 1 and 2 as many times as necessary until bubbles rise out of the dip tube.

Cultivation

Removing residual fluid

To remove residual fluid from the system, proceed as follows:

Procedure:



1. Hold the syringe with sample downwards, pull back the plunger.

This removes all but a few μL of the residual fluid.



2. Hold the sample valve with one hand; unscrew the syringe with the other.

3. If desired: Place the closing caps on the sample valve and on the syringe with the sample.

9.3 Inoculation

Check and ensure the following items before inoculation:

- Medium has been filled.
- Heat-labile, separately sterilized substances are present.
- The reagent bottles are connected to the pumps and the culture vessel and are filled with reagents and nutrient solution enough for the duration of the entire cultivation.
- The hoses of the reagent bottles are filled.

- The correct operating temperature has been reached.
- The required stirring speed is set.
- The sensors are calibrated, and the control is set correctly (maybe not active yet).
- All clamps have been removed (except for sampling system).
- Utensils for the inoculation and vessels with inoculum are ready.

Methods

There are a number of ways to add medium or inoculum before and during cultivation:

- In a small volume, with the syringe via the septum
- Via the addition port adapter from the reagent bottle (a sterile hose connection is required for this method).
- Via the dip tube from the reagent bottle (a sterile hose connection is required for this method).

These methods are described below.

The implements for inoculation with a syringe are standard accessories for the device. This inoculation method is particularly suitable for all vessel sizes of the device.

9.3.1 Inoculation with a Syringe

Proceed as follows for the inoculation:

Procedure

1. Fill the syringe with the required amount of inoculum.
2. Unscrew the blanking plug from the septum collar.
As a possible additional protection against contamination:
Before piercing, drop a few drops of ethanol (70 %) on the septum.
3. Pierce the septum and inject the inoculum.
4. Remove the needle from the septum and close the septum collar with a blanking plug.

9.3.2 Inoculation Using Dip Tube / Addition Port Adapter

Proceed as follows during inoculation:

Procedure

1. Fill the inoculum under sterile conditions into the prepared container.
2. Create a sterile hose connection with the dip tube/addition port adapter.

Cultivation

3. Transfer the desired volume of inoculum into the culture vessel. Pump it, if necessary.
4. Clamp off the hose by means of a clamp, weld it if necessary.



INFORMATION

An inoculation needle WITHOUT septum collar and WITHOUT septum can be used like an addition port adapter or a dip tube.

9.4 Harvest

The culture can be harvested at the end of the cultivation. To prevent possible sedimentation from the culture, the stirrer can be switched on during harvesting. If necessary, activate gassing for sensitive cultures. However, all other parameters should be switched off, provided there are no other specifications for the user.

The following possibilities exist for the harvest:

- a) Transfer to another vessel
To transfer the contents of the vessel to another container in a laminar flow cabinet.
- b) Pump-down via a sterile hose connection
To do so, proceed as follows:

Procedure

1. Make a sterile connection between the hose at the dip tube for harvest and the new vessel.
2. Connect the hose to one of the pumps on the device or to an external pump.
3. Pump the desired amount of culture into the new vessel.



INFORMATION

Only switch on the stirrer, if it is fully covered by medium, as foam otherwise forms.

4. Switch off all parameters on the operating panel, i.e. stop the bioreactor.



ATTENTION

Switching the device off at the power switch without stopping the bioreactor and shutting down the system on the operating panel beforehand may lead to damage of the operating panel!

9.5 Emptying the Culture Vessel

Depending on the user specifications, the culture vessel can be emptied either before or after autoclaving.

A previously emptied and culture vessel filled only with water for autoclaving is easier to clean afterwards.

For emptying the culture vessel, the same options as for harvesting are available. For more information, see chapter "Harvest".

If the culture will not be used further, it must be inactivated according to the current in-house instructions (e.g. by autoclaving or by lowering the pH value), and subsequently disposed of in an environmentally sound manner according to the local regulations.

9.6 Emptying the Reagent Hoses



ATTENTION

Residues of acids and alkalis in the reagent hoses during autoclaving can damage the pump heads.

- Completely empty all reagent hoses before autoclaving.
- Thoroughly rinse the reagent hoses with water after emptying.

Before autoclaving the culture vessel with accessories, all reagent hoses must be completely emptied via the corresponding pump. This can either be done using the rocker switches of the pumps on the basic unit or via the touch screen software.



INFORMATION

When using several devices at the same time, it is useful and time-saving to empty all reagent hoses simultaneously and automatically.

For details about emptying via touch screen software refer to the separate operating manual of the touch screen software.

Cultivation

9.7 Switching off the Device

When the harvest is finished or the culture vessel has been emptied and the reagent hoses are also empty, the device can be switched off.

Proceed as follows:

Procedure

1. Ensure that the bioreactor has been stopped. If necessary, stop it in the touch screen software on the operating panel.
2. Shutdown the system on the operating panel.
3. Switch off the device at the power switch.



ATTENTION

Switching the device off at the power switch without previously stopping the bioreactor and shutting down the system on the operating panel may lead to damage of the operating panel!

4. Close the supply lines (water, gas).
5. Autoclave the vessel, built-in parts and accessories as per the user-specific specifications and then clean them.

9.8 Autoclaving the Culture Vessel after Cultivation

After emptying the culture vessel and before cleaning, the culture vessel must be autoclaved with all accessories.

When doing so, do not autoclave the culture vessel when completely dry and observe the same safety regulations as when autoclaving before cultivation.

Before starting, ensure:

- There is liquid in the culture vessel (autoclavable medium or approx. 10 mL water per liter working volume).
- Reagents and feed solution have been pumped back out of the hoses.
- The device is switched off.

Proceed as follows to prepare the culture vessel and accessories for autoclaving after cultivation:

Procedure

1. Clamp off the hoses of the reagent bottles.
2. Clamp off the hose of the sparger.
3. Remove all cable and hose connections between the basic unit and the culture vessel:
 - c) Unplug the sensor cables.
 - d) Pull the temperature sensor out of the immersion pocket.
 - e) Disconnect the water inlet and water outlet hoses of the exit gas cooler from the basic unit.
 - f) Remove the gassing hose(s) (emerging from basic unit) from the inlet air filter(s).
4. Lightly cover all filters with aluminium foil.



ATTENTION

DO NOT cover **DIGITAL** pH and pO₂ sensors with aluminium foil!

5. Open the pump cover.
6. Remove the mounting plate with pump heads from the drive shafts on the basic unit and fit to the vessel holder.
7. Release snap closure between thermal blocks and pull off the culture vessels in its holder from the basic unit.
8. Check and ensure that the exit gas filter is free and dry and the exit gas hose is **OPEN**.
9. Insert the temperature sensor of the autoclave into the immersion pocket on the culture vessel and autoclave the culture vessel.

Cleaning and Maintenance

10 Cleaning and Maintenance

The following sections describe in detail how the culture vessel and accessories and the basic unit are cleaned and, as required, stored.

In addition, the section contains a maintenance plan and corresponding descriptions for the procedures to be performed by the operator.

10.1 Cleaning Agent and Disinfectant

Intended use	Allowed products/tools
Culture vessel	Water and a non-scratch, non-abrasive sponge or washing-up brush; lab washer with special washing agent (for industry and lab use)
Cleaning agent for denaturation of proteins	0.1 N NaOH
Cleaning agent for smaller component parts	Ultrasonic bath
Cleaning agent for surfaces	Water
Disinfectant for surfaces	Ethanol, 70 %
Decalcifier for the device	Amidosulfonic acid (in liquid form)

Cleaning and Maintenance

10.2 Cleaning the Culture Vessel - Routine Cleaning

The culture vessel and accessories can be cleaned as soon as they have cooled down after autoclaving.



ATTENTION

Household washing-up liquid and soap (in particular cream soaps) can collect in glass pores and impair later cultivations.

Never clean culture vessels and accessories with household soap and use special cleaning agent (for industrial and lab use) in the lab washer.

The following method describes a routine cleaning between two cultivations. It takes place with the culture vessel completely assembled and the accessories completely mounted.

This does not include the sensors, with the exception of antifoam or level sensors from the device manufacturer. To avoid damaging the other sensors during the routine cleaning, they are first removed and then cleaned separately according to the third-party manufacturer guidelines and then stored, if necessary. Also see the “Removing Sensors” section and “Cleaning Sensors”.

Proceed as follows to carry out a routine cleaning of the culture vessel:

Procedure

1. Carefully unscrew the sensors (except antifoam/level sensors) by hand (no tools!) from the vessel top plate ports and place them to the side for separate cleaning according to the manufacturer guidelines.
2. Completely fill the culture vessel with 0.1 N NaOH.
3. Fit the top plate on the vessel and secure it with the clamping ring with quick-release fastener.
4. Insert the vessel holder with the culture vessels from above into the thermal blocks on the basic unit and fix it.
5. Switch on the device on at the power switch.
6. At the operating panel in the touch screen software, start the bioreactor and stir strongly for 2 hours with the stirrer function (parameter *Stirrer*).



INFORMATION

It is recommended to warm the 0.1 N caustic soda to 60 °C and to prolong the duration of stirring for dealing with persistent residue of foam or protein.

Cleaning and Maintenance

7. Stop the bioreactor in the touch screen software at the operating panel.
8. Shutdown the system at the operating panel.
9. Switch the device off at the power switch.
10. Remove the top plate and place it so that it does not(!) lie on top of built-in parts.
11. Empty the culture vessel.
12. Thoroughly rinse the culture vessel with distilled water.

10.3 Removing the Vessel Top Plate and Accessories

All accessories must be removed for thorough cleaning of the individual parts of the culture vessel. This is described in the following sections. The cleaning itself is described in the chapter “Cleaning and Storing Individual Parts”.

The cleaning of the hoses with pump heads, the basic unit and the operating panel are described in separate sections.


Sensors from third-party manufacturers are cleaned according to their manufacturer's specifications.


10.3.1 Removing the Exit Gas Cooler

To remove the exit gas cooler, proceed as follows:


Procedure

1. Unscrew the exit gas cooler from the vessel top plate port by hand.
Ensure that the O-ring does not get lost.
2. Remove the pressure hose with exit gas filter, dispose of the exit gas filter.
3. Unscrew and remove the coupling nut on the lid by hand in counter-clockwise direction.

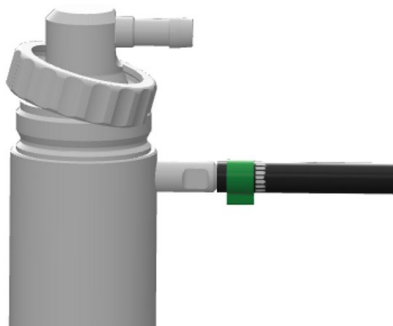

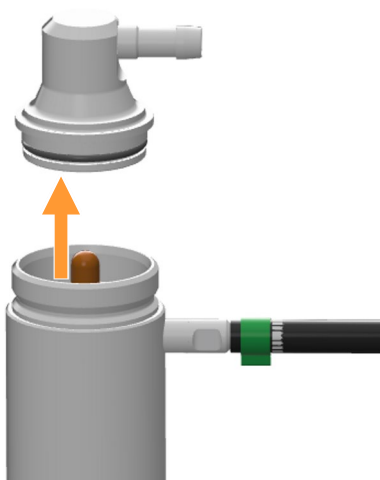Cleaning and Maintenance


4. Remove the lid by hand.
If necessary, wet the lid slightly with water to facilitate loosening of the lid.

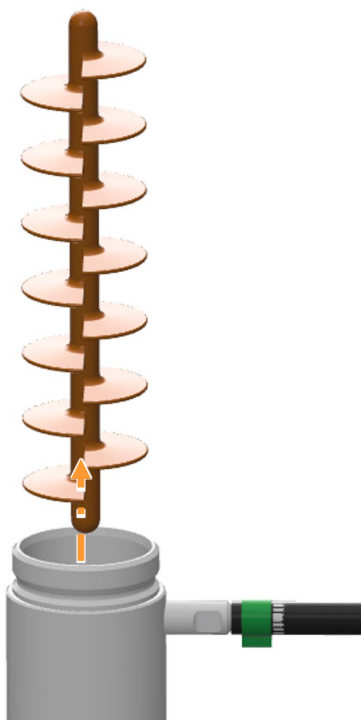

5. Remove the silicone baffle from the exit gas cooler.

6. Clean the individual parts of the exit gas cooler. For details on cleaning, see chapter "Cleaning and Storing Individual Parts".

Cleaning and Maintenance

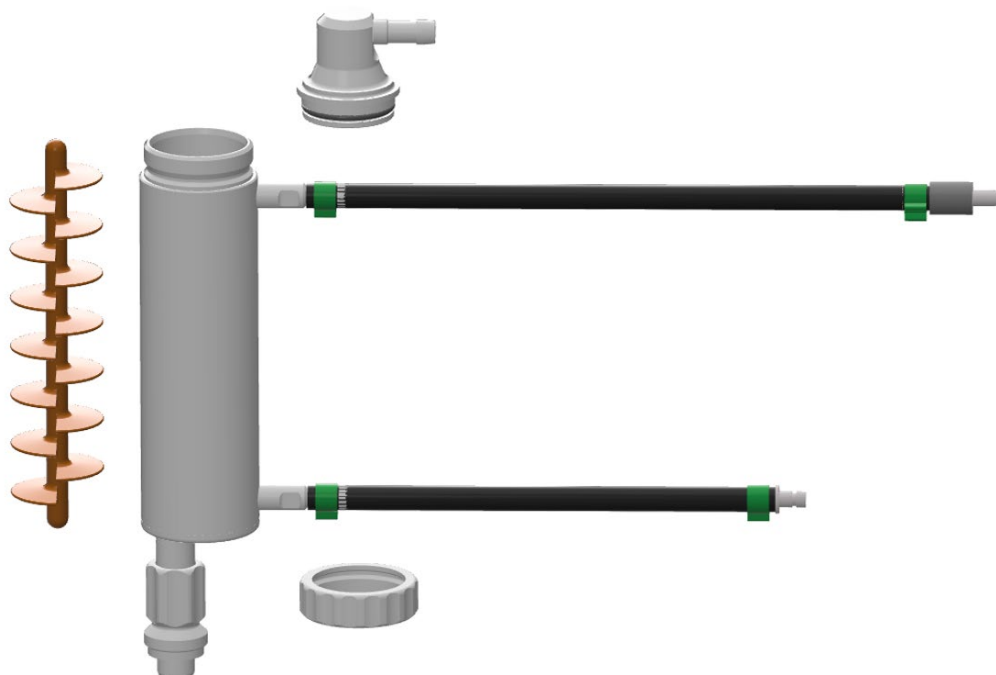

INFORMATION

For 400 mL culture vessels, the exit gas cooler is screwed into the adapter sleeve, which is screwed into the 12 mm/Pg13.5 port together with the O-ring due to space constraints. Both parts can also be screwed out of the port or the adapter sleeve by hand.

10.3.2 Removing the Sensors

Sensors are either mounted directly into the ports or by means of a sensor holder or clamping adapter. For removal of the sensors, proceed as follows:

Sensors without holder/clamping device

Procedure

1. Carefully unscrew the sensor by hand (no tools!) from the vessel top plate port.

Sensor with sensor holder

Procedure

1. Carefully loosen and unscrew the sensor on the hollow screw of the sensor holder from the port by hand.
2. Carefully unscrew the sensor from the guide bar and gently pull it out of the sensor holder.

Cleaning and Maintenance

Procedure

Sensor with clamping adapter (antifoam and level sensor)

1. Loosen slotted screw(s) next to the sensor in the port.



INFORMATION

This step is only necessary for the type of clamping adapter for 10 mm ports. Clamping adapters for 12 mm / Pg13.5 ports can be directly unscrewed from the port.

2. Carefully pull out or unscrew the clamping adapter together with the sensor from the port by hand.
3. Ensure the O-ring of the clamping adapter does not get lost.
4. Loosen the slotted screw on the clamping adapter and carefully pull the sensor out of the clamping adapter by hand.
5. Ensure that the insulation on the sensor does not get damaged.

10.3.3 Removing Hoses, Filters and Pump Heads

To later clean reagent hoses and pump heads, they must be removed from the reagent bottles and from components of the culture vessel.



INFORMATION

To avoid damage, never dismantle the pump heads. Always replace a damaged pump head along with the pump hose, and vice versa.

Proceed as follows:

Procedure

1. Remove cable ties (e.g. with a side cutter) so that the hoses are not damaged.
2. Pull hoses off the culture vessel and the reagent bottles.
3. Remove and dispose of filters for pressure equalization and hoses from reagent bottles.
4. Ensure that the inlet air filter is clean, dry and not blocked. If this is not the case, dispose of it.



INFORMATION

If the filter for pressure equalization and the corresponding hoses have been used several times, ensure that the filters are always dry and clean.

Cleaning and Maintenance

5. Dispose of the exit gas filter (see also chapter “Removing the Exit Gas Cooler”).

10.3.4 Removing Blanking Plugs

Proceed as follows:

Blanking plugs in 10 mm ports

Procedure

1. Loosen the slotted screw(s) next to the blanking plug in the port.
Ensure the screw(s) does/do not get lost.
2. Pull the blanking plug out of the port by hand.
Ensure that the O-ring on the blanking plug does not get lost.

Blanking plugs in 12 mm/Pg13.5 ports

Procedure

1. Loosen the blanking plug with the hexagon socket spanner and remove it by hand.
Ensure that the O-ring does not get lost.

Blanking plugs in 7.5 mm ports



INFORMATION

The procedure remains the same as for the addition port adapters in the 7.5 mm ports.

Procedure

1. Unscrew the hose holder from the bearing holder and remove it.
2. Pull the blanking plug out of the port by hand.
Ensure that the O-ring on the blanking plug does not get lost.

10.3.5 Removing the Septum Collar and the Septum

Proceed as follows:

Procedure

1. Unscrew the septum collar out of the port by hand.
2. Remove the septum from the port and dispose of it.

10.3.6 Removing the Vessel Top Plate




INFORMATION


Treat the clamp, top plate and vessel as one unit so that the same clamp is always used for the same top plate and the same vessel.

To remove the vessel top plate, proceed as follows:

Procedure

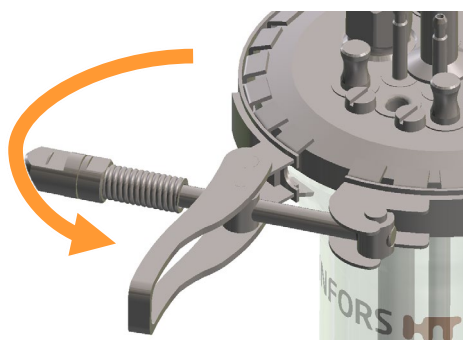

1. Hold the vessel on the clamping ring with one hand and open the fastening with the other hand.

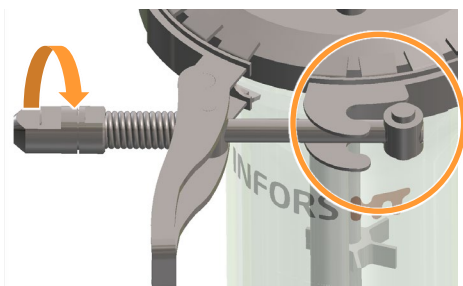

2. Use one hand to tighten the clamping ring and use the other to turn and unhook the threaded rod.

3. Remove the clamping ring from the top plate.
4. Carefully lift the top plate out of the glass vessel and put it down on the top plate side so that it cannot put pressure on built-in-parts.

10.3.7 Removing the Immersion Pocket for Temperature Sensor (Pt100)

Proceed as follows:

Procedure

1. Loosen the slotted screw(s) next to the port and ensure the screw(s) do/does not get lost.
2. Push the immersion pocket from the inside of the vessel top plate up, so that it can be pulled out of the port from the outside of the top plate.

Ensure the O-ring on the immersion pocket does not get lost.

Cleaning and Maintenance

10.3.8 Removing the Sparger and Dip Tube

Straight spargers and dip tubes can generally be removed from the outside of the vessel top plate. Curved spargers and dip tubes can only be removed from the inside of the vessel top plate.

Since this equipment uses curved spargers and straight dip tubes, removal from the inside of the vessel top plate is described here. This means that the vessel top plate has already been removed.



INFORMATION

Before removing the sparger, we recommend measuring and recording the position to aid correct mounting at a later stage.

Proceed as follows:

Procedure

1. Loosen the slotted screw on the clamping adapter.
2. Carefully pull the sparger/dip tube from the bottom out of the clamping adapter.
3. Loosen the slotted screw(s) next to the port and ensure that it is/they are not lost.
4. Pull the clamping adapter out of the port from the vessel top plate. Ensure that the O-ring is not lost.

10.3.9 Removing the Baffles

To remove the baffles, proceed as follows:

1400 mL culture vessel: two-piece baffles

Procedure

1. Loosen the slotted screws on the baffles.
2. Remove both baffles from the bearing holder.
Make sure you do not lose the slotted screws; if appropriate, screw the two halves of the baffles together for cleaning.

750 mL culture vessel: one-piece baffles

The baffles consist of one piece and are welded to the bearing holder. Removal takes place in the same way as for the bearing holder, see chapter “Removing the Bearing Holder”.

Cleaning and Maintenance**10.3.10 Removing the Hose Holder and Addition Port Adapters**


To remove the hose holder and the addition port adapters, proceed as follows:

Procedure

1. Pull the hose holder wire from the hose holder and set it aside.
2. Unscrew the hose holder from the bearing holder in the top plate; use a wrench if necessary.
3. Pull the addition port adapters from the ports by hand.
Ensure that the O-rings on the addition port adapters are not lost.


10.3.11 Removing the Stirrer Shaft

The stirrer shaft can be removed if necessary. To do so, proceed as follows:

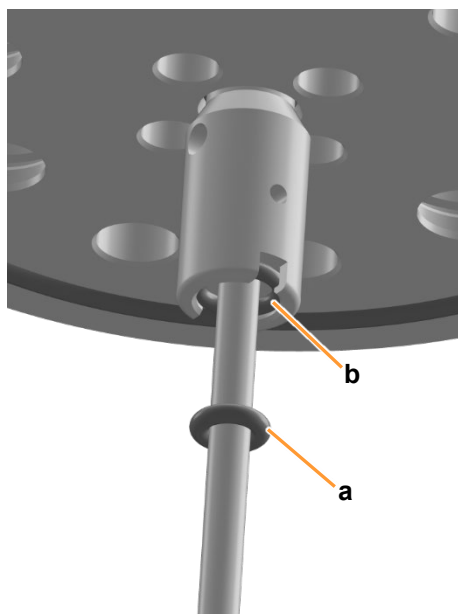
Procedure

1. Slightly pull down the small O-ring (a) on the stirrer shaft.
2. Carefully push out to upper, larger O-ring (b) from the groove in the bearing holder; if necessary, use a small key/pin (not sharp or sharp-edged).

Cleaning and Maintenance

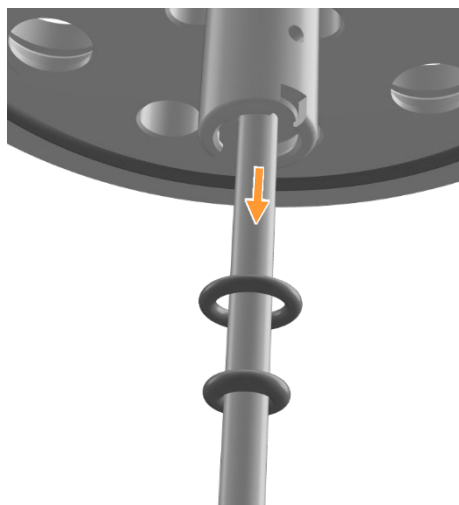

3. Carefully pull the stirrer shaft out of the bearing holder.

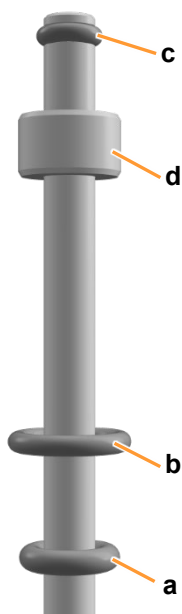

4. Ensure that the three O-rings (a – c) and the stirrer shaft bearing (d) are not lost.

10.3.12 Removing the Magnetic Coupling, Flow Deflector and Impeller




ATTENTION

Danger of material damage caused by magnetic fields. Magnetic fields can damage laptops, hard drives, ATM cards, data media and other items susceptible to magnetism.


Before removing the individual parts, we recommend measuring and recording their positions to facilitate correct remounting later.

Cleaning and Maintenance


To remove the magnetic coupling, the flow deflector and impellers from the stirrer shaft, proceed as follows:

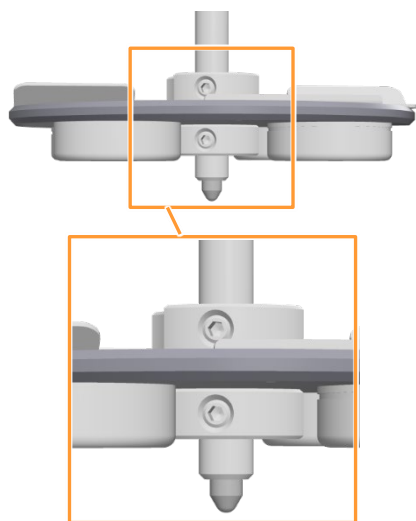Procedure

1. Loosen the grub screws on both adjusting rings below and above the magnetic coupling.

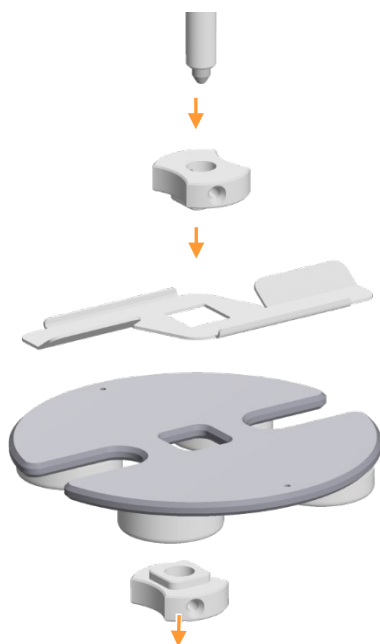


2. Remove the lower adjusting ring, magnetic coupling, flow deflector and upper adjusting ring from the stirrer shaft.

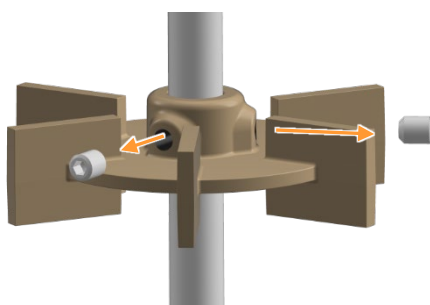

3. Loosen the grub screws on the impellers.

Cleaning and Maintenance

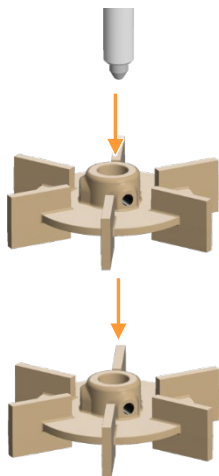

4. Remove the impeller from the stirrer shaft.




INFORMATION

Make sure no individual parts are lost for later assembly after cleaning.

10.3.13 Removing the Bearing Holder

To remove the bearing holder from the vessel top plate, proceed as follows:

Procedure

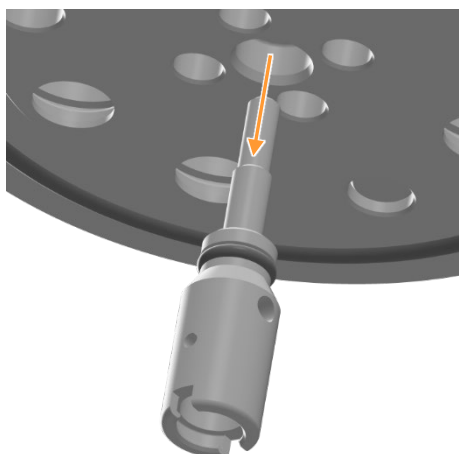

1. Pull the bearing holder out of the top plate from below.



INFORMATION

The bearing holder is held firmly in place in the top plate due to the O-ring. If necessary, wiggle the bearing holder a little while pulling it out to loosen the O-ring.

Cleaning and Maintenance

10.4 Cleaning and Storing Individual Parts

The procedure described here is suitable for the following individual parts:

- Vessel
- Exit gas cooler
- Accessories such as blanking plugs, spargers, dip tubes, addition port adapters etc.
- Reagent bottles
- Vessel top plate



INFORMATION

The cleaning of the sensors, hoses and pump heads as well as the basic unit and the exit gas cooler is described in separate chapters.

Special information on the centering bearing



ATTENTION

Loss of the centering bearing!

The centering bearing in the aeration ring of the sparger or in the triangular plate can fall out of the holder during cleaning in the dishwasher and thus be lost!

Depending on the level of contamination and internal cleaning requirements, carefully clean the triangular plate or the sparger by hand.

Special information on the magnetic coupling

If so-called flash rust has formed on the magnetic coupling during the autoclaving process due to the adhesion of ferromagnetic particles, it can be placed in a citric acid solution for cleaning. For details, see chapter "Cleaning the Magnetic Coupling".

Special information on the vessel top plate

If the vessel top plate is to be cleaned in the dishwasher, we recommend removing the stirrer shaft.

To clean the individual parts, proceed as follows:

Procedure

1. Clean parts using distilled water and a soft sponge or clean them in the dishwasher.

Cleaning and Maintenance

Ensure that any deposits in the dip tubes and exit gas cooler are removed. Use 0.1 N caustic soda solution and then follow up with distilled water as necessary. For this, see chapter “Cleaning the Culture Vessel”.

2. Dry all parts, including the insides of the dip tubes, sparger and the exit gas cooler including its hoses for water inlet/outlet.
3. Check all O-rings for cracks or damage. Replace them if necessary.
4. Store the vessel, vessel top plate and accessories in a clean, dry state in a location where they cannot be physically damaged (e.g. by falling), or prepare them for the next cultivation as necessary.

10.5 Cleaning the Sensors

Apart from antifoam and level sensor, all sensors are cleaned and maintained according to the descriptions of the sensor manufacturer.

Procedure

1. Clean the sensors according to the sensor manufacturer guidelines.
2. Prepare the sensors for the next cultivation or, if necessary, service and/or store them according to the sensor manufacturer guidelines.

10.6 Cleaning the Hoses and Pump Heads

Proceed as follows to clean the reagent hoses and pump heads:

Procedure

1. Thoroughly rinse the hoses with the pump heads with water.
2. Carefully dry all hoses and, if necessary, blow out with clean-compressed air.



INFORMATION

To avoid damage, never dismantle the pump heads. Always replace a damaged pump head along with the pump hose, and vice versa.

Cleaning and Maintenance

10.7 Cleaning the Super Safe Sampler



ATTENTION

Risk of damage to the sampling system from unsuitable cleaning methods or cleaning agent (such as acids, bases or solvents, for example).

- Only use water or a mild soap solution for cleaning.
- The sterile filter must remain dry at all times.

Proceed as follows to clean the sampling system:

Procedure

1. Fill the culture vessel with water or a mild soap solution.
Or: Remove the sampling hose from the dip tube and hold it in a vessel, e.g. a beaker, with water or a soap solution.
2. Place the syringe on the automatic valve and pull out the plunger to rinse the sampling system.
When using a soap solution:
3. Then rinse the sampling system thoroughly with water.



INFORMATION

If the test record requires that the culture is killed off after cultivation by autoclaving the culture vessel, the valves of the sampling system may become stuck due to residue of the culture solution. In such a situation, it would be better to autoclave the sampling system separately in a beaker of water (hoses filled with water, filter removed).

10.8 Cleaning the Magnetic Coupling

Due to the very strong magnets in the magnetic coupling at the lower end of the stirrer shaft, ferromagnetic particles can be deposited on the stainless steel surfaces of the magnetic coupling. These particles are often not visible to the human eye. During autoclaving of the culture vessel, they decompose and cause visible stains, so-called flash rust.

Stains created in this way can be removed by a simple cleaning procedure.

Prepare the following:

- Produce 5 % citric acid cleaning solution with demineralised water and citric acid.

Cleaning and Maintenance

- Provide a vessel (glass, plastic) for inserting the magnetic coupling.

Proceed as follows for cleaning:

Procedure

1. Remove the magnetic coupling from the stirrer shaft.
2. Place the magnetic coupling in the vessel with the magnets facing upwards.
3. Fill the vessel with the cleaning solution so that the magnetic-coupling is completely covered with liquid.
4. Leave the vessel with the magnetic coupling in place for at least 12 hours.
If required, this time can also be extended up to 24 hours.
5. After the exposure time, remove the magnetic coupling from the solution and check visually:
 - If stains are still detected, the procedure can be repeated.
 - Particularly persistent stains can be removed with an abrasive sponge.



INFORMATION

After using the abrasive sponge, the cleaning procedure in the acid bath must be repeated so that a protective layer can form again.

Preventive measures

The procedure with the citric acid cleaning solution can also be carried out directly in the culture vessel before autoclaving. This means that the stirrer shaft and all the necessary built-in-parts are mounted and the vessel top plate is in place. The vessel top plate should not be removed after the cleaning procedure. Emptying and rinsing of the culture vessel should take place via a port in the vessel top plate. This prevents the stirrer shaft, respectively the magnetic coupling from coming into contact with ferromagnetic particles again before autoclaving.

Cleaning and Maintenance

10.9 Cleaning the Basic Unit and Operating Panel

Proceed as follows to clean the surface of the basic unit and the operating panel as required:

Procedure

1. Switch off the device at the power switch.
2. Disconnect the device from the power supply.
3. Wipe all surfaces with a damp cloth.
Clean with an appropriate disinfectant as necessary.
4. Clean the screen with a wipe suitable for computer or laptop screens.

10.10 Maintenance Plan



WARNING

Non-compliance of this maintenance plan contains a high risk!

It is the responsibility of the user, that this maintenance plan is complied with. Non-compliance will lead to exclusion of liability (see General Terms and Conditions).

The required maintenance for reliable operation is described in the following chapters.

Reduce the maintenance intervals in case increased abrasion is detected during regular checks.

Contact the manufacturer for questions concerning maintenance.

Cleaning and Maintenance

To be carried out by operator

Interval	Maintenance work
Before each cultivation	Check all hoses and hose connections, replace hoses if necessary. Have supply hoses replaced by qualified personnel.
	Check the fit and soundness of the centering bearing in the triangular plate or the aeration ring of the sparger (750 mL vessel).
	Check cables for damage and kinks.
	Check that all O-rings and gaskets are leak-proof, replace if necessary.
	Check the integrity of all glass parts (vessel, reagent bottles) and replace if necessary.
	Check all filters and replace if necessary. Replace the exit gas filter.
	If necessary, calibrate the sensors.
After every cultivation	Autoclave and clean the culture vessel and accessories.
As required	Clean the basic unit and operating panel.
	Replace the centering bearing.

To be carried out by qualified personnel

Interval	Maintenance work
Every 6 months	Check functionality of measurement sections (temperature, pH, etc.), use simulator, where possible.
As required	Replace supply hoses.

To be carried out by operator, ONLY AFTER CONSULTATION OF MANUFACTURER

Interval	Maintenance work
As required	Decalcify the device.

To be carried out by INFORS HT service technician

Interval	Maintenance work
Annually (recommendation)	Full maintenance of the device.

Cleaning and Maintenance

10.11 Decalcifying the Device

Calcification could block built-in parts, lines or valves in the basic unit. It may be necessary to decalcify the device if certain faults occur in the temperature control system.

Note the following points, before beginning the procedure:



ATTENTION

Inappropriate decalcifying of the device may lead to loss of property.

Only decalcify the device **AFTER CONSULTATION** of the manufacturer or licensed dealer!

- Carry out decalcification of the basic unit with both bioreactors running in parallel.
- Be sure to respect the in chapter “Technical Data” specified inlet pressure.
- To warm up the decalcifier and pump it into the basic unit, use a chiller or a water bath and an external pump.
- During decalcification, the decalcifier flows in a circuit between the basic unit and the chiller/water bath.
- Use amidosulfonic acid in liquid form as decalcifying agent.



ATTENTION

Amidosulfonic acid can crystallise in case of overdosage and cause loss of property!

When preparing the decalcifying liquid, observe and follow the manufacturer's instructions for correct dosage and application!

- For the mixture, calculate 5 liters of water plus the capacity of the water bath/chiller including the hoses.

Proceed as follows for decalcifying:

Procedure

1. Connect both culture vessel in their holder to the basic unit and fixate them by means of the snap closure between the thermal blocks.
2. Mount both exit gas coolers to the vessel top plates of both culture vessels and connect them to the basic unit.
Ensure that the valves for the exit gas cooler water supplies are open. Open them, if necessary.
3. Fill the chiller/water bath with the prepared decalcifying liquid.

Cleaning and Maintenance

4. Connect the chiller or water bath to the water inlet and outlet on the basic unit using hoses.
5. To open the corresponding valves in the basic unit, set the temperature on the operating panel to 5 °C (cool).
6. Set the chiller/water bath to 20 °C to 40 °C.
7. Switch on the pump at the chiller/water bath.
8. Let the decalcifier flow through the device for an hour.
9. Connect the water inlet hose on the device to tap water.
10. Hang the water outlet hose of the device at the spout.
11. Rinse the device for an hour.


10.12 Replacing the Centering Bearing

If the centering bearing is lost, damaged or loose, it must be replaced.


Proceed as follows:

400 mL and 1400 mL TV vessels

Step

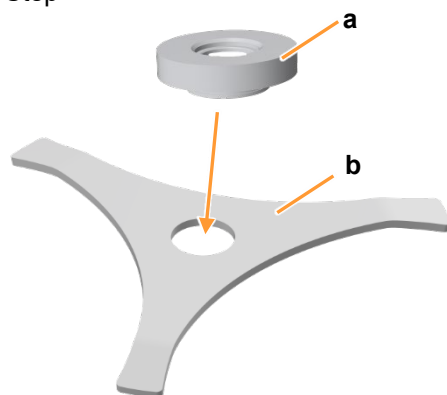


Gently press the centering bearing (a) into the groove in the triangular plate (b) with your finger.

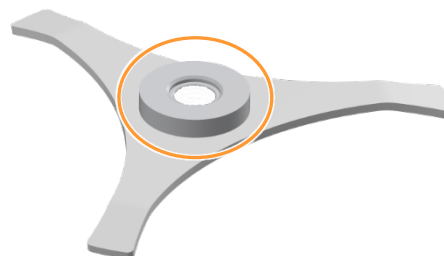


750 mL vessels

Step

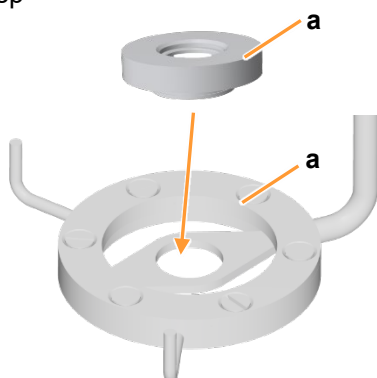

Gently press the centering bearing (a) into the groove in the aeration ring (b) with your finger.

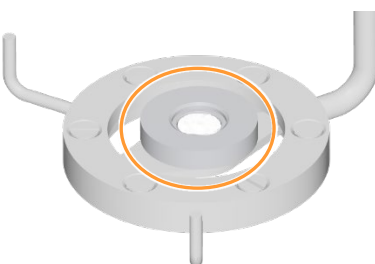

11 Interferences

The following section describes possible reasons for interferences and how to resolve them. Reduce the service intervals in correspondence with the actual loads if interferences become increasingly common. Contact the manufacturer or licensed dealer for interferences that cannot be resolved by following the above instructions.

11.1 Interferences Basic Unit and Operating Panel

Interference		
Device does not work. Power switch is not illuminated; screen of the operating panel remains dark.		
Possible cause	Remedy	By
Device is not switched on.	Switch on the device at the power switch.	Operator
Power supply of the device is interrupted.	■ Check if the plugs are connected ■ Check the mains connection.	Operator
Device fuse is blown.	Replace the fuse. If the fault occurs more than once, contact the INFORS HT representative.	Operator

Interference		
Power switch is illuminated; screen of the operating panel remains dark.		
Possible cause	Remedy	By
Monitor of operating panel is switched off.	Press the ON/OFF key on the monitor.	Operator
Power supply cable of the operating panel is not connected.	Connect the power supply cable to the DC connection of the operating panel.	Operator

Interference		
No communication between device and operating panel.		
Possible cause	Remedy	By
Display cable is not connected.	Connect the display cable: Plug the round connector in at the COM1 connection of the operating panel. Plug the flat connector in one of the two iDDC-bus connections on the rear side of the basic unit.	Operator

Interferences

11.2 Drive System Interferences

Interference		
Stirrer does not start.		
Possible cause	Remedy	By
The <i>Stirrer</i> parameter is not activated.	Activate the parameter.	Operator
<i>Stirrer</i> parameter setpoint = 0.	Set setpoint > 0.	Operator
The pO_2 parameter is activated and set to oxygen control via the stirrer (cascade).	Switch cascade off and test function via the <i>Stirrer</i> parameter.	Operator

Interference		
Motor control is volatile, irregular or stops.		
Possible cause	Remedy	By
Incorrect PID settings in the <i>Stirrer</i> parameter	Reset the PID settings to default values.	Operator

Interference		
Unusual sounds when the stirrer is running.		
Possible cause	Remedy	By
The impeller touches other built-in-parts in the culture vessel or the stirrer shaft does not sit correctly in the centering bearing.	Stop the bioreactor, shut down the system and switch off the device. Correctly mount built-in-parts under consideration of internal safety regulations. Check the fit of the stirrer shaft and adjust its end clearance if necessary.	Operator
The centering bearing has come off the triangular plate or the aeration ring or the ceramic part is broken.	Replace the centering bearing.	Operator

Interferences

11.3 Interferences Temperature Control System

Interferences		
No temperature control.		
Possible cause	Remedy	By
Temperature control is not activated.	Switch parameter <i>Temperature</i> on.	Operator
Stirrer is not activated and/or set-point = 0.	Switch parameter <i>Stirrer</i> on and enter setpoint > 0, as required.	Operator

Interference		
No heating or inadequate heating: thermal block in the basic unit does not get hot even with a high temperature set point		
Possible cause	Remedy	By
Thermal block has overheated (automatic over-temp.cut out.)	Wait for unit to cool. Mechanical cut out in basic unit should re-set automatically.	Operator

Interference		
No cooling or inadequate cooling.		
Possible cause	Remedy	By
No water supply or inadequate flow.	Check the water supply and turn the supply tap if necessary.	Operator
Incorrect Negative factor in option <i>PID</i> of parameter <i>Temperature</i>	Check Negative factor: Value must be positive. Adjust as necessary.	Operator

Interference		
Temperature fluctuations		
Possible cause	Remedy	By
Incorrect PID settings parameter <i>Temperature</i>	Check PID settings and adjust as necessary, especially <i>P-term</i> .	Operator

Interferences

11.4 Interferences Gassing System

Interferences		
No gassing / air bubbles in the culture vessel.		
Possible cause	Remedy	By
The on-site gas supply has been interrupted.	Stop the bioreactor. Check the on-site gas supply and switch it on, if necessary.	Operator
Depending on the configuration of the gassing system: The rotameter valve(s) is/are not open. And/or: The <i>Flow</i> parameter(s) is/are not activated. And/or: Setpoint in the <i>Flow</i> parameter(s) = 0. Or: Parameter <i>GM Flow</i> = 0 and/or <i>GasMix</i> is/are not activated.	Slowly open the rotameter needle valve(s). And/or: Activate the <i>Flow</i> parameter(s). And/or: Set the setpoint(s) in the <i>Flow</i> parameter(s) > 0. Or: Set parameter <i>GM Flow</i> > 0 and activate parameter <i>GasMix</i> .	Operator
Hose connection(s) between the basic unit and the culture vessel is/are kinked or clamped.	Check whether the hose connection(s) is/are clamped; if necessary open the clamp(s). Check hose connection(s) for kinks, if necessary, route them again or replace them under observation of the sterility requirements.	Operator
Inlet air filter is blocked.	Replace the inlet air filter under sterile conditions.	Operator

Interference		
The desired gas flow rate is not reached.		
Possible cause	Remedy	By
Blocked holes on the sparger.	Stop the bioreactor and clean the sparger.	Operator

Interferences

Interference		
Sudden increase in evaporation losses in the culture vessel.		
Possible cause	Remedy	By
The exit gas cooler does not cool. The valve for water flow is closed.	Open the valve.	Operator
The exit gas cooler does not cool, parameter <i>Temperature</i> is activated.	Check the water supply to the exit gas cooler. Restore it, if necessary. The basic unit is calcified. Decalcify the device, if necessary.	Operator

11.5 Interferences pH Control

Interference		
No display or incorrect display of pH, digital measurement systems: the message ERROR is displayed instead of the current value.		
Possible cause	Remedy	By
Sensor cable not connected or not properly connected.	Connect properly if necessary.	Operator
<u>Analog measurement system:</u> <i>Temp. Compens.</i> (temperature compensation) is switched off.	Switch the function <i>Temp. Compens</i> on in Setpoint option of parameter <i>pH</i> .	Operator
pH drift during long cultivation.	Recalibrate pH with external measured values, respectively perform a product calibration.	Operator
Faulty pH sensor.	Test calibration with pH 4 and pH 7 buffer. <u>Digital measurement systems:</u> Note the error message(s) (<i>Show Sensor Status</i>) when calling up the calibration menu. Regenerate or replace the sensor. Consult the documentation of the sensor manufacturer!	Operator

Interferences

Interference		
No pH control.		
Possible cause	Remedy	By
Parameter <i>pH</i> is not activated.	Activate the parameter.	Operator
Incorrect dead band setting.	Check the dead band (Dead Band in PID settings): Switch off or enter a small value.	Operator
No addition of reagents (acids and base).	Check the reagent bottles: Refill if necessary. Check the hose connections between the reagent bottles and the culture vessel: Connect properly if necessary. Open/remove hose clamps if necessary.	Operator
Pump(s) (base/acid) do/does not operate properly.	Check operation using the rocker switch.	Operator
Pump hose is damaged.	Replace pump head.	Operator
Incorrect hose type connected.	Replace if necessary.	Operator

Interference		
pH value drifts up and down over time or acid and base are added almost continuously in turn.		
Possible cause	Remedy	By
Incorrect PID setting in <i>pH</i> parameter.	Check the PID settings and adjust as necessary. Change the special proportional factor (<i>Prop. Term</i>) or <i>Dead band</i> setting.	Operator
Incorrect strength of reagents: Concentration is too weak or too strong.	Check the strength of reagents. Adjust if necessary: 0.1 mol to 2.0 mol.	Operator

Interferences

11.6 Interferences pO₂ Control

Interferences		
No display or incorrect display of pO ₂ . Digital measurement systems: the message <i>ERROR</i> is displayed instead of the current value.		
Possible cause	Remedy	By
Sensor cable is not connected or not properly connected.	Connect the sensor cable properly.	Operator
Analog measurement system: pO ₂ sensor is not polarised.	Polarise the pO ₂ sensor	Operator
Faulty pO ₂ sensor.	Check the calibration of the pO ₂ sensor. <u>Digital measurement systems</u> : Note the error message(s) (<i>Show Sensor Status</i>) when calling up the calibration menu. Replace the sensor if necessary. Consult the documentation of the sensor manufacturer!	Operator

Interference		
No pO ₂ control.		
Possible cause	Remedy	By
The pO ₂ parameter and/or cascaded parameter is/are not activated.	Activate parameters.	Operator
The cascade settings are incorrect.	Check the cascade settings and change as necessary.	Operator.
No gas flow into culture vessel.	Refer to interferences in the gassing system.	Operator

Interference		
Unstable pO ₂ control.		
Possible cause	Remedy	By
Incorrect PID settings in the pO ₂ parameter.	Check the PID settings (<i>PID</i> parameter option) and adjust as necessary. Special proportional factor (<i>Prop. Term</i>) and dead band. Dead band value must be 0 (zero).	Operator

Interferences

11.7 Interferences Antifoam or Level Sensor and Antifoam Pump

Interference		
Foam/medium is not detected.		
Possible cause	Remedy	By
Sensor is not properly connected.	Check connections and connect properly as necessary.	Operator

Interference		
Foam/medium is always/frequently detected.		
Possible cause	Remedy	By
Insulation of sensor is damaged.	Have the sheathing of the sensor replaced. For this, contact INFORS HT representative.	INFORS HT service technician

Interference		
Antifoam pump does not work.		
Possible cause	Remedy	By
Parameter <i>Antifoam</i> is not activated.	Activate the parameter.	Operator
Dosing time of parameter <i>Antifoam</i> = 0 (zero).	Set dosing time > 0.	Operator

Interference		
No antifoam agent or medium supply or inadequate flow.		
Possible cause	Remedy	By
Reagent bottle is empty.	Refill if necessary.	Operator
Wrong antifoam agent or incorrect concentration.	Replace if necessary.	Operator
Hose line blocked or clamped.	Check the hose connection between the reagent bottle and the culture vessel: If necessary, connect them correctly. Open/remove clamps if necessary.	Operator
Antifoam pump does not work.	Check operation using the rocker switch.	Operator
The pump hose is damaged.	Replace pump head.	Operator
Incorrect hose type connected.	Replace if necessary.	Operator

11.8 Interferences Feed and Pump

Interference		
No addition of nutrient solution ("Feed") or inadequate addition.		
Possible cause	Remedy	By
Parameter <i>Feed</i> is not activated.	Activate the parameter.	Operator
Setpoint of parameter <i>Feed</i> = 0.	Set setpoint > 0.	Operator
Reagent bottle is empty.	Refill if necessary.	Operator
Hose line blocked or clamped.	Check the hose connection between the reagent bottle and the culture vessel: If necessary, connect them correctly. Open/remove clamp if necessary.	Operator
Feed pump does not work.	Check operation using the rocker switch.	Operator
The pump hose is damaged.	Replace pump head.	Operator
Incorrect hose type connected.	Replace if necessary.	Operator

11.9 Replacing Device Fuses




INFORMATION

Device fuses may only be replaced by fuses of the same rating. For detailed information concerning the requirements for the fuses refer to main chapter "Technical Data", chapter "Connection Values", "Electrical".

To replace a defective device fuse, proceed as follows:

Procedure

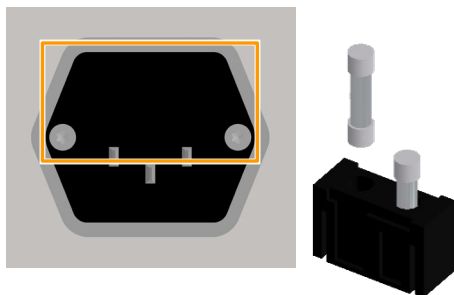

1. Switch off the device and pull out the power plug.
2. Unlock the plug for the fuses by pressing together the two flaps and pull out the plug at the same time.
3. Remove the defective fuse.
4. Insert a new fuse with the correct number of Amperes.
5. Push the plug as far back in the opening as possible until it snaps in.
6. Re-establish the power supply to the device.

Interferences

11.10 Behavior in Case of Power Interruption

If the power supply to the device is interrupted during a running cultivation process (e.g. by turning off at the power switch or in case of a power failure), all parameter setpoints are stored.

After the power supply is restored, an interrupted cultivation process is automatically continued with the last stored setpoints.

The fact that a power interruption has occurred is indicated by the system alarm *Restart after power failure*. However, the duration of the event cannot be determined from the alarm.

11.11 Returning for Repair

The provider must return the device or the faulty component part(s) to the manufacturer if, after consulting the service department of the local dealer or the manufacturer, on-site diagnosis and/or repair is not possible.



INFORMATION

When returning the device, the component part or accessory for repair, it is required for the safety of all parties involved and because of legal provisions that a lawful declaration of decontamination is present. Refer to main chapter “Safety and Responsibility”, chapter “Declaration of Contamination” for details.

12 Disposal

Once the end of use has been reached, the device must be dismantled and disposed of in an environmentally friendly manner. The materials must be disposed of in accordance with national and local legislation. The local municipal authority or specialist waste disposal companies can provide information on environmentally friendly disposal.

If no special return arrangements have been agreed, INFORS HT devices can be returned to the manufacturer or licensed dealer for disposal with the required declaration of decontamination. For further details refer to main chapter "Safety and Responsibility", chapter "Declaration of Contamination".



WARNING

Electronic waste, electronic components, lubricants or other auxiliary materials/supplies are subject to hazardous waste regulations and may only be disposed of by registered specialist disposal firms.



Disposal Information in accordance with the WEEE Directive (2012/19/EU)


The device is marked with the symbol of a crossed-out wheeled bin in accordance with Directive 2012/19/EU on waste electrical and electronic equipment (WEEE). This symbol indicates that the device must not be disposed of with household waste. To prevent environmental damage and health risks caused by improper disposal, the device must be taken to a separate collection point for electrical and electronic equipment at the end of its service life.

Technical Data

13 Technical Data


13.1 Dimensions

13.1.1 Master Device and Satellite Devices

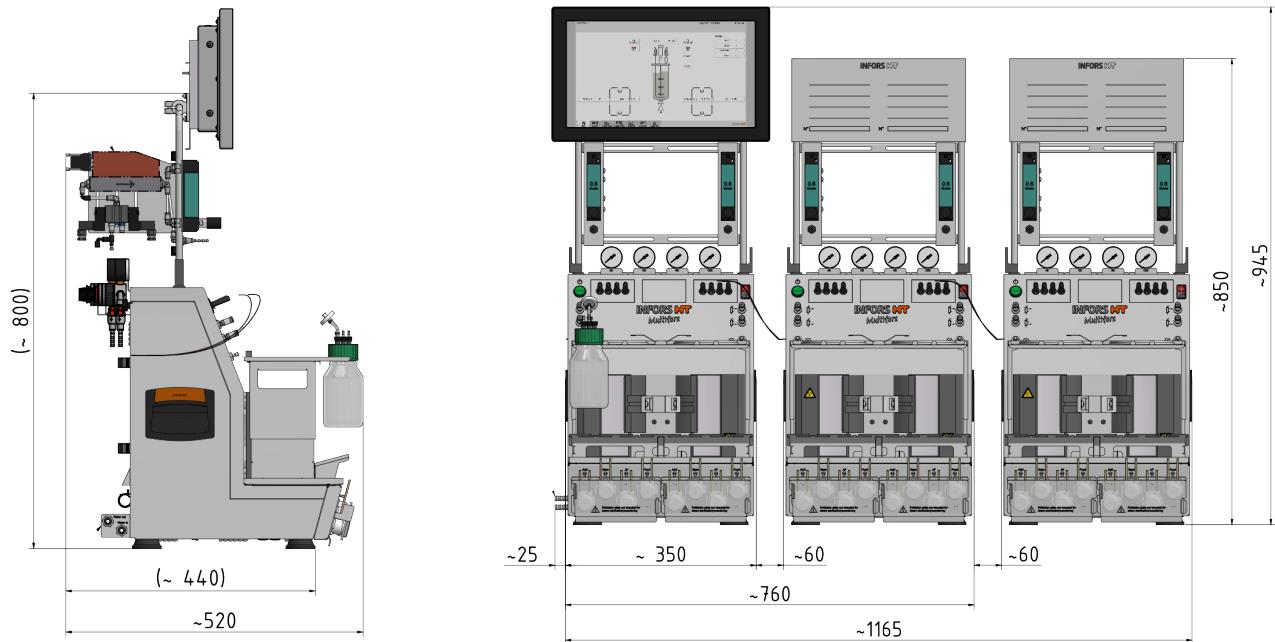

All dimensions in mm

13.1.2 Culture Vessels in Vessel Holder

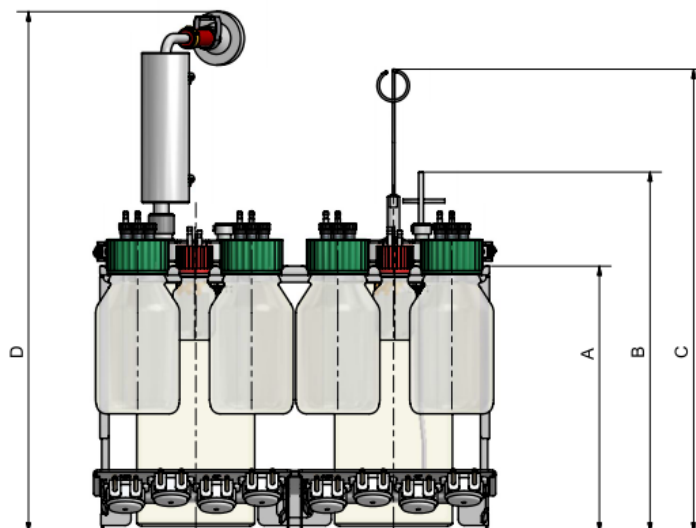


The height of the vessel holder is adjustable.

Dimensions	Vessels (Total Volume)		
	400 mL	750 mL	1400 mL
A	182 mm	196 mm	222 mm
B	260 mm	274 mm	300 mm
C	350 mm	364 mm	390 mm
D	395 mm	409 mm	435 mm

Technical Data

Top view

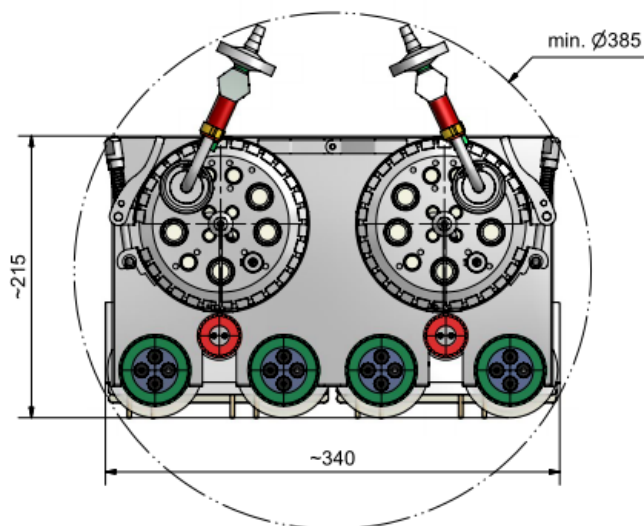

Dimensions in mm, applies to all vessel sizes.

13.2 Weights

Description	Value	Unit
Touch screen operating panel	5	kg
Basic unit with 2 culture vessels (with standard fittings) and operating panel	approx. 40	kg

13.3 Connection Values

13.3.1 Electrical

Description	Type 230 V	Type 115 V	Unit
	Value		
Voltage	230	115	V
Frequency range	50 / 60	60	Hz
Max. current	4	8	A
Fuses (5 x 20 mm, slow-blown)	4	8	A

Technical Data

13.3.2 Water IN

Description	Value	Unit
Connection pressure	2 ± 1	bar
Temperature min.	+1	°C
Connection: OD of hose nozzle	8.3	mm

13.3.3 Water OUT

Description	Value	Unit
Connection pressure	No back pressure	
Temperature max. (also with optional heating 90 °C)	80	°C
Connection: OD of hose nozzle	8.3	mm

13.3.4 Gas(es) IN

Description	Value	Unit
Connection pressure	2 ± 0.5	bar
Connection: OD of hose nozzle	7	mm
General gas quality	Dry, clean and free of oil and dust	
Recommended compressed air quality	class 1.2.1 As per DIN ISO 8573-1	

13.3.5 Exit Gas

Description	Value	Unit
Connection pressure	No back pressure	
Connection: OD of hose nozzle	8	mm

Technical Data

13.4 Specifications

13.4.1 Operating Panel

Description	Value
HMI	Color touch screen 15.6"
Protection	IP 66

13.4.2 Culture Vessels

Description	Value	
Form	Cylindrical with flat bottom	
Material	Glass vessel	Borosilicate glass
	Top plate and built-in parts	316L, electropolished ¹⁾
	O-rings	EPDM

¹⁾ Exceptions: impellers in 750 and 1400 mL culture vessels and stirrer shaft bearings of all vessel sizes. For details refer to Stirrer.

Vessel sizes

TV ¹⁾	WV max. ²⁾	WV min. ³⁾	DN ⁴⁾ mm	Height mm
400	250	115	70 / 55	181
750	500	180	70	195
1400	1000	320	90	220

¹⁾ Total volume in mL

²⁾ Min. working volume in mL

³⁾ Max. working volume in mL

⁴⁾ Nominal diameter = inner diameter vessel

Ports in vessel top plate

Ø mm	Thread	Number acc. to vessel size		
		400 mL TV	750 mL TV	1400 mL TV
7 mm	Without	4	4	4
10 mm	Without	4	4	4
12 mm	Pg13.5	3	4	5

Technical Data

13.4.3 Stirrer

Description	Value	
Drive	Magnetic	
Motor	Typ: DC, external rotor motor Nominale power: 56 W ¹⁾ Nominal torque: 90 mNm ¹⁾	
Range of rotation speed with 2 impellers ²⁾	400 mL vessels	100 min ⁻¹ to 1600 min ⁻¹
	750 mL vessels	100 min ⁻¹ to 1500 min ⁻¹
	1400 mL vessels	100 min ⁻¹ to 1500 min ⁻¹
Accuracy Measurement	± 5 min ⁻¹ at ≤ 1000 min ⁻¹ 1 % setpoint at > 1000 min ⁻¹	
Accuracy Control	≤ ± 5 min ⁻¹ at ≤ 1000 min ⁻¹ ≤ 1 % setpoint at > 1000 min ⁻¹	
Direction of rotation stirrer shaft	Counter-clockwise (top view vessel)	
Bearing housing material	Ceramic, Teflon	


¹⁾ At max. rotation speed

²⁾ With water at 30 °C, and 0.5 vvm air flow sparger

Impellers



Type / Number / Material	Vessel
6-bladed impeller (90°), 2 pieces, 316L, electro polished	400 mL
Rushton impeller, 6 blades, 2 pieces, Peek	750 mL and 1400 mL

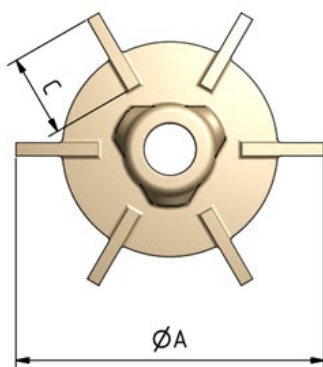

Vessel	A	B	C
400 mL	24 mm	6,5 mm	4.8 mm
750 mL	30 mm	8.0 mm	8.0 mm
1400 mL	38 mm	9.0 mm	11.0 mm

Technical Data

13.4.4 Temperature

Description	Value	
Heating	Electrical, thermal block 315 W	
Cooling	With tap water or chiller via Thermal block	
Sensor	Type: Pt100 1/3 DIN-B	
Measurement range	0 °C to +145 °C	
Control range	from 5 °C above inlet temperature	
	Standard	to 70 °C
	Option	to 90 °C
Accuracy measurement and control	$\pm 0,3 \text{ °C}$ at $\leq 60 \text{ °C}$: $\pm 0,5 \text{ °C}$ at $> 60 \text{ °C}$:	

13.4.5 Gassing

General	
Gas entry	Sparger
Specific gassing rates	2 min ⁻¹ ¹⁾
Gas(es)	Air / Air + O ₂ / Air + N ₂ / Air + O ₂ + N ₂ / CO ₂ ²⁾

¹⁾ Calculated for max. working volume for all vessel sizes

²⁾ Optional for pH control via sparger

Gassing strategy variant “Basic”	
Gas flow control	1 rotameter
Accuracy rotameter	$\pm 5 \%$
Gasmix control (if available)	1 solenoid valve per gas

Gassing strategy variants “Standard” and “High End”		
Gas flow control	Standard	1 MFC ¹⁾
Accuracy rotameter	High End	1 MFC per gas
Gas flow accuracy	Measurement	$\pm 1.5 \%$ FS
	Control	$\leq \pm 1.5 \%$ FS
Gasmix control (if available)	Standard	1 solenoid valve per gas
	High End	Via MFCs

¹⁾ Mass flow controller

Technical Data

Measurement ranges MFC and rotameter in L min⁻¹

Max. working volume vessel	Rotameter "Basic"	MFC "Standard" and "High End"	MFC CO ₂ (sparger, pH control)
0.25 L	0.08 to 0.6	0.005 to 0.5	0.0025 to 0.25
0.5 L	0.1 to 1	0.01 to 1	0.005 to 0.5
1 L	0.3 to 2	0.02 to 2	0.01 to 1



INFORMATION

The mass flow controllers are calibrated by their manufacturer ex works at standard conditions, i.e. at 1.013 bar and 20 °C. Therefore, for every gas flow rate the gas volume flow is given in L min⁻¹.

13.4.6 Antifoam

Description	Value
Sensor	Conductive with dosing needle, adjustable mounting depth
Control	Peristaltic pump <i>Antifoam</i>
Display	0 (no foam) / 100 (foam)

13.4.7 pH Control

Description	Value
Control	Peristaltic pumps <i>Acid</i> and <i>Base</i> or with CO ₂ instead of acid.
Control range	pH 2 to 12
Measurement accuracy	pH ± 0.1

Technical Data

Variants of measurement systems

Measurement system analog		
Traditional pH sensor (potential measurement against reference)		
Variant METTLER	Sensor type	405-DPAS-SC-K8S/120
	Measurement range	pH 2 to 12
Measurement systems digital		
Traditional pH sensor (potential measurement against reference) with integrated electronics		
Variant HAMILTON	Sensor type	Easyferm Plus ARC
	Measurement range	pH 0 to 14
Variant METTLER	Sensor type	InPro 3253i, ISM
	Measurement range	pH 0 to 14



INFORMATION

pH sensors type Easyferm Plus ARC are preconfigured by the device manufacturer INFORS HT. Replacement sensors must be configured before use.

Details about technical data, use and maintenance of the pH sensors are in the separate documentation from the sensor manufacturers.

13.4.8 pO₂ Control

Description	Value
Control	Via cascade: Stirrer, gas flow, gasmix, O ₂ addition. <i>The functionality of the parameters depends on the hardware configuration of the device.</i>
Control range	0 %-sat to 100 %-sat
Measurement accuracy	1 % FS

Technical Data

Variants of measurement systems

Measurement system analog

Traditional amperometric/polarographic pO₂ sensor

Variant METTLER	Sensor type	InPro 6820/25/080
	Measurement range	0 % sat to 150 %-sat

Measurement systems digital

pO₂ sensor with integrated optical electronics

Variant HAMILTON	Sensor type	Visiferm RS485-ECS
	Measurement range	0 %-sat to 300 %-sat
Variant METTLER	Sensor type	InPro6860i, ISM
	Allowed temperature range	0 °C to 60 °C
	Measurement range	0 %-sat to 285 %-sat



INFORMATION

Digital pO₂ sensors are pre-configured from the device manufacturer INFORS HT. Replaced sensors must be configured again before use!

Details about technical data, use and maintenance of the pO₂ sensors are in the separate documentation from the sensor manufacturers.

13.4.9 Pumps

Description	Value	
Type	Peristaltic	
Standard	Digital	Acid Base Antifoam
	Analog	Feed
Rotation speed	Digital	74 min ⁻¹ / fixed rotation speed
	Analog	74 min ⁻¹ / max. rotation speed, adjustable within range of 0 % to 100 %
Accuracy	± 1 % FS	

Technical Data

Pump hoses and flow rates

Description	Value
Material	PharMed BPT
Standard	iD: 1.0 mm Wall thickness: 1.1 mm Flow rate: 3.5 ml min ⁻¹
Option 1	iD: 0.5 mm Wall thickness: 1.15 mm Flow rate: 1.2 ml min ⁻¹
Option 2	iD: 2.5 mm Wall thickness: 1,0 mm Flow rate: 17.2 ml min ⁻¹
Flow rates	All flow rates at 74 min ⁻¹ (100 % rotation speed)

13.5 Operating Conditions

Description	Value
Ambient temperature	5 °C up to 40 °C
Relative air humidity, non-condensing	20 % up to 90 %
Altitude operating location	max. 2000 m.a.s.l
Degree of pollution (as per EN 61010-1)	2
Min. distance from walls, ceilings and other appliances	150 mm

13.6 Emissions

Description	Value	Units
Noise emission	<70	dB (A)

13.7 Auxiliary Supplies

pH Buffers

pH buffers are used to calibrate the pH sensors. 250 mL bags are available for the following buffers:

- pH 4.04
- pH 7.01

14 EC-Declaration of Conformity

EG-Konformitätserklärung

EC-Declaration of conformity

Déclaration CE de conformité

INFORS HT

Infors AG, Headoffice, Switzerland
Rittergasse 27, CH-4103 Bottmingen
T +41 (0)61 425 77 00
info@infors-ht.com, www.infors-ht.com

Gemäss der EG-Maschinen-Richtlinie 2006/42/EG, Anhang II 1 A

In accordance with directive on machinery 2006/42/EC, appendix II 1 A

D'après la directive relative aux machines 2006/42/CE 2006, annexe II 1 A

Hersteller <i>Manufacturer</i> <i>Fabricant</i>	Infors AG Rittergasse 27 CH-4103 Bottmingen
Bezeichnung <i>Designation</i> <i>Désignation</i>	Tischbioreaktor Bench-top bioreactor Bioréacteur de paillasse
Typ <i>Type</i> <i>Type</i>	Multifors 2
Ab Release <i>From release</i> <i>A partir du version</i>	alle Releases all releases toutes les versions
Ab Seriennummer <i>From serial number</i> <i>A partir du numéro de série</i>	S-000127197

Dieses Gerät entspricht den grundlegenden Anforderungen der Richtlinien

This device is in compliance with the essential requirements of directives
Cet appareil est conforme aux exigences essentielles des directives

Maschinenrichtlinie 2006/42/EG	Directive on machinery 2006/42/EC	Directive relative aux machines 2006/42/CE
EMV-Richtlinie 2014/30/EU	EMC directive 2014/30/EU	Directive CEM 2014/30/UE

Aussteller
Issuer
Editeur

Bevollmächtigter für die technische Dokumentation
Person authorised to compile the technical file
Person autorisée à constituer le dossier technique



C. Rutishauser

Infors AG
Rittergasse 27
CH-4103 Bottmingen
Anschrift
Address
Adresse

Konformitätsbeauftragter
Representative for conformity
Responsable de la conformité



M. Heuschkel
Chief Technology Officer

Bottmingen, 16. Nov. 2021
Ort, Datum
Place, date
Lieu, date

